

K3NH Temperature Meter




Operation Manual

Produced January 1998

Notice:

OMRON products are manufactured for use according to proper procedures by a qualified operator and only for the purposes described in this manual.

The following conventions are used to indicate and classify precautions in this manual. Always heed the information provided with them. Failure to heed precautions can result in injury to people or damage to the product.

-  **DANGER** Indicates information that, if not heeded, is likely to result in loss of life or serious injury.
-  **WARNING** Indicates information that, if not heeded, could possibly result in loss of life or serious injury.
-  **Caution** Indicates information that, if not heeded, could result in relatively serious or minor injury, damage to the product, or faulty operation.

OMRON Product References

All OMRON products are capitalized in this manual. The word “Unit” is also capitalized when it refers to an OMRON product, regardless of whether or not it appears in the proper name of the product.

The abbreviation “Ch,” which appears in some displays and on some OMRON products, often means “word” and is abbreviated “Wd” in documentation in this sense.

The abbreviation “PC” means Programmable Controller and is not used as an abbreviation for anything else.

Visual Aids

The following headings appear in the left column of the manual to help you locate different types of information.

Note Indicates information of particular interest for efficient and convenient operation of the product.

1, 2, 3... 1. Indicates lists of one sort or another, such as procedures, checklists, etc.

© OMRON, 1998

All rights reserved. No part of this publication may be reproduced, stored in a retrieval system, or transmitted, in any form, or by any means, mechanical, electronic, photocopying, recording, or otherwise, without the prior written permission of OMRON.

No patent liability is assumed with respect to the use of the information contained herein. Moreover, because OMRON is constantly striving to improve its high-quality products, the information contained in this manual is subject to change without notice. Every precaution has been taken in the preparation of this manual. Nevertheless, OMRON assumes no responsibility for errors or omissions. Neither is any liability assumed for damages resulting from the use of the information contained in this publication.

TABLE OF CONTENTS

PRECAUTIONS	xi
1 General Precautions	xii
2 Safety Precautions	xii
3 Application Precautions	xii
4 Noise Prevention	xiii
SECTION 1	
Introduction	1
1-1 Features	2
1-2 Front of the Meter	3
1-3 Rear of the Meter	6
1-4 Modes	7
1-5 Communications Function	8
1-6 Field Calibration	8
SECTION 2	
Setup	9
2-1 Mounting	10
2-2 Input Block	11
2-3 Output Board	14
SECTION 3	
Parameter Setting	19
3-1 Overview	20
3-2 Setting Mode	21
3-3 Protect Mode	58
SECTION 4	
Operations in RUN Mode	67
4-1 Displaying and Changing Setting Values	68
4-2 Displaying and Resetting of Maximum and Minimum Values	71
4-3 External Input Signals	72
SECTION 5	
Useful Functions	73
5-1 Teaching Function	74
5-2 Output Test	76
5-3 Maintenance Mode	77
SECTION 6	
BCD Output	93
6-1 Connectors	94
6-2 Timing Charts	97
SECTION 7	
Troubleshooting	99
7-1 Items to Be Checked First	100
7-2 Display	100

TABLE OF CONTENTS

Appendices

A Specifications	103
B Available Models	107
C List of Settings	109
D Available Parameters	111

Index	113
--------------------	------------

Revision History	117
-------------------------------	------------

About this Manual:

This manual describes the installation and operation of the K3NH Temperature Meter and includes the sections described below.

Please read this manual carefully and be sure you understand the information provided before attempting to install and operate the K3NH.

Section 1 describes the functions of the K3NH. The main components are also described.

Section 2 provides instructions required for mounting and wiring the K3NH.

Section 3 provides instructions for setting the parameters of the K3NH.

Section 4 provides instructions for operating the K3NH in RUN mode.

Section 5 provides information on the teaching function, output test, and maintenance mode.

Section 6 provides information on the use of the K3NH with the BCD Output Board.

Section 7 provides information for troubleshooting the K3NH

The **Appendices** provide specifications, a list of settings, a list of standard models, and a list of available menu items.



WARNING

Failure to read and understand the information provided in this manual may result in personal injury or death, damage to the product, or product failure. Please read each section in its entirety and be sure you understand the information provided in the section and related sections before attempting any of the procedures or operations given.

PRECAUTIONS

This section provides precautions for using the K3NH Temperature Meter and related devices.

The information contained in this section is important for the safe and reliable application of the K3NH. You must read this section and understand the information contained before attempting to set up or operate the K3NH.

1 General Precautions	xii
2 Safety Precautions	xii
3 Application Precautions	xii
4 Noise Prevention	xiii


1 General Precautions


The user must operate the product according to the performance specifications described in the operation manuals.

Before using the product under conditions which are not described in the manual or applying the product to nuclear control systems, railroad systems, aviation systems, vehicles, combustion systems, medical equipment, amusement machines, safety equipment, and other systems, machines, and equipment that may have a serious influence on lives and property if used improperly, consult your OMRON representative.

Be sure to read this manual before attempting to use the product and keep this manual close at hand for reference during operation.

2 Safety Precautions

 **WARNING** Never attempt to disassemble any Units while power is being supplied. Doing so may result in serious electrical shock or electrocution.

 **WARNING** Never touch any of the terminals while power is being supplied. Doing so may result in serious electrical shock or electrocution.

3 Application Precautions

Observe the following precautions when using the product.

- Always use the power supply voltage specified in the specifications.
- Do not use the product in locations subject to flammable gases or combustible objects.
- Be sure to confirm terminal names when wiring.
- Be sure to tighten the screws on the terminal blocks.

Observe the following precautions when mounting the product.

- Mount the product on level surfaces.
- Mount the product on a panel which has a thickness of 1 to 3.2 mm.


Do not mount the product in the following places.

- Locations subject to strong shock or vibration.
- Locations subject to temperature or humidity exceeding the rated levels or where icing is liable to occur.
- Locations subject to dust.
- Locations subject to corrosive gases (particularly sulfuric gases or ammonium gases).
- Locations subject to direct sunlight or outdoor conditions.
- Locations near devices (high-frequency welders or high-frequency sewing machines) that produce high-frequency noise.


4 Noise Prevention

Provide the following countermeasures when using the product in an environment where the product is exposed to noise.

- Countermeasures for protecting the product against high-frequency noise or abnormal voltages.

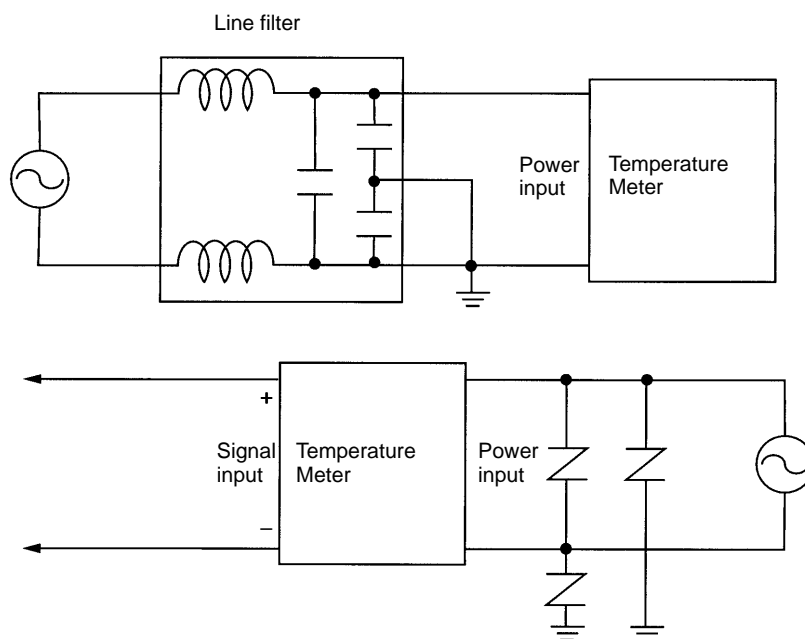

- Countermeasures for protecting the product against inductive noise produced from the input line.

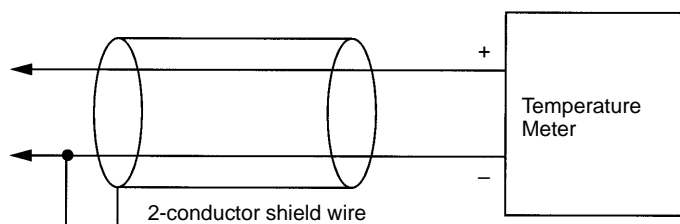

SECTION 1

Introduction

This section describes the functions of the K3NH. The main components are also described. Refer to the remaining sections of this manual for the operation of the K3NH and its menus in detail.

1-1	Features	2
1-2	Front of the Meter	3
1-3	Rear of the Meter	6
1-4	Modes	7
1-5	Communications Function	8
1-6	Field Calibration	8

1-1 Features

The K3NH Temperature Meter displays temperature input.

The K3NH has the following functions.

Scaling

Refer to page 31. Sensor voltage or current output is converted into a value within a specified range.

Comparative Output Selection

Comparison output patterns can be selected from the standard, level, or zone output depending on the application.

Refer to *Comparative Output Patterns*, page 48.

Linear Output

Refer to *Linear Output Range*, page 53.

BCD Output

A digital data output format where every four binary bits is numerically equivalent to one decimal digit.

Refer to *Section 6 BCD Output*.

Communications Output

Refer to the *K3NH Communications Manual*.

HOLD

HOLD is an external input which is used to stop the A/D process and freeze the display. The comparative, linear, and BCD outputs are also retained.

Refer to *4-3 External Input Signals* for details.

RESET

RESET is an external input to reset the present maximum and minimum values. The process value when the RESET is ON is set as the maximum and minimum values. The maximum and minimum values can be reset using the front panel keys.

Refer to *4-2 Displaying and Resetting of Maximum and Minimum Values*.

Teaching

The K3NH is provided with a teaching function that can set an actual measured value as a setting value without key input.

This function is useful for setting parameters while checking the operating status of the K3NH.

The teaching function can be used to set the set and scaling values. It can be also used to set the linear output range of the K3NH with a Linear Output Board.

Refer to *5-1 Teaching Function* for details.

Output Test

This function is convenient for checking a system to which the K3NH is connected, especially when some inputs cannot be operated. The K3NH simulates an input to check the output conditions.

Refer to *5-2 Output Test* for details.

Standby Sequence

When the K3NH is tuned on, the K3NH will have no output until the measured value is within the PASS range. This function avoids unnecessary output until the output is within the measurement range after the power is turned ON.

Hysteresis

The established setting value includes a hysteresis setting to prevent “chattering” of the output when the measured value fluctuates in the vicinity of the setting values.

Hysteresis is enabled when the measured value starts to become smaller than the HH and H setting values and larger than the LL and L setting values.

Refer to *Hysteresis*, page 46.

Remote/Local Selection

The K3NH can be operated remotely through a host computer or locally with key inputs.

Remote Mode: For programming remotely by downloading setup parameters from a host computer via RS-232C.


Local Mode: Programming is performed with the front panel key input.

Refer to *Remote/Local Programming*, page 56.

Average Processing

Average processing prevents the display from fluctuating due to unstable input. Simple average processing or movement average processing can be selected. Refer to *Average Processing*, page 39.

1-2 Front of the Meter

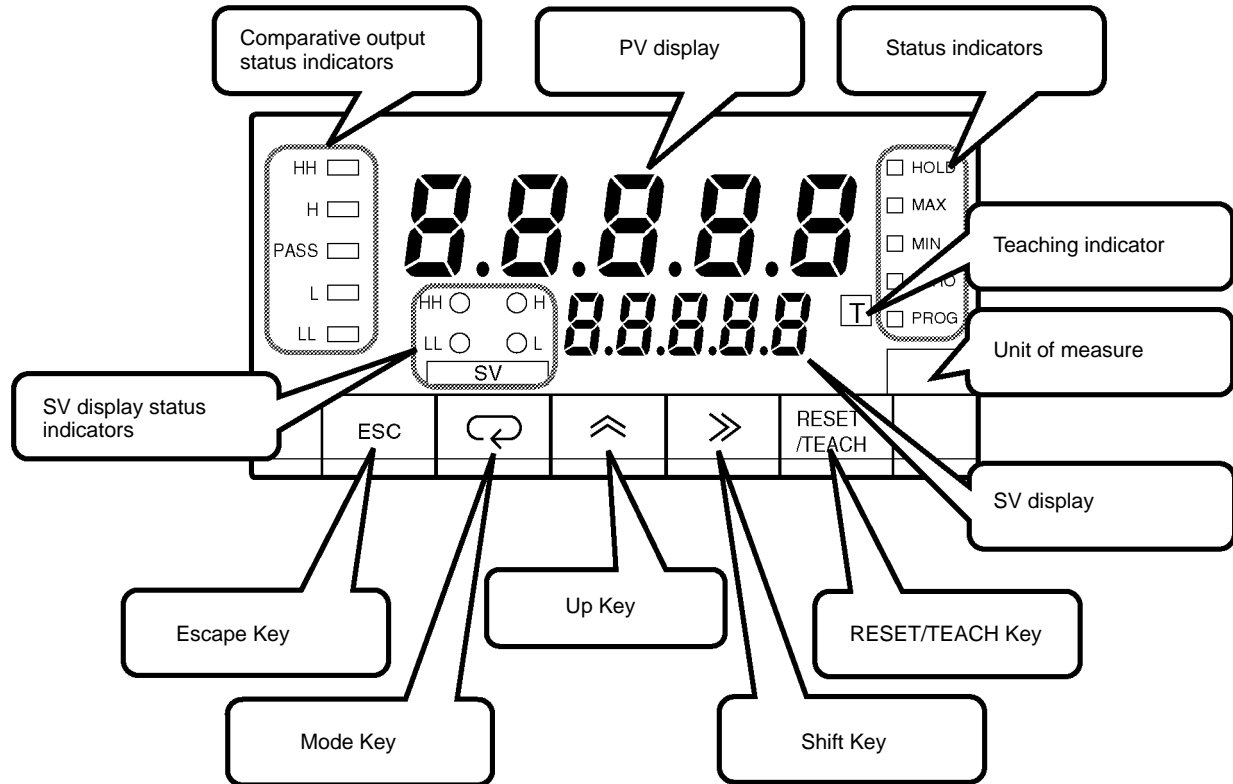

Five-digit (–19999 to 99999), seven-segment, 14.2-mm-high LED display with a programmable decimal point.

The displays show the process value, maximum value, minimum value, operations/parameters when setting, and error messages.

PV Display

K3NH-□□□A Basic Model

RUN Mode: Displays the process, maximum, and minimum values. Also displays setting values while the SV indicator is lit. When changing a value, all digits other than those that can be set become dimmer.

Setting Mode: Displays the menu, parameter, or setting value. When changing a value, all digits other than those that can be set become dimmer.

K3NH-□□□C Set Value LED Display Model

RUN Mode: Displays the process, maximum, and minimum values.

Setting Mode: Displays the menu and parameters.

SV Display (Setting value LED Display Models Only)

RUN Mode: Displays comparative setting values. When changing a value, all digits other than those that can be set become dimmer.

Setting Mode: Displays setting values. When changing a value, all digits other than those that can be set become dimmer.

Comparative Output Status Indicators

Indicates the status of the comparative output.

Status Indicators**HOLD Indicator**

Lit when the HOLD input signal is ON.

MAX Indicator

Lit when the value displayed on the PV display is the maximum value.

MIN Indicator

Lit when the value displayed on the PV display is the minimum value.

PROG Indicator

Lit when the setting mode menu is displayed. The indicator flashes while parameters are displayed.

Teaching Indicator

Lit when displayed parameters can be set in teaching operation. The indicator flashes when the process value is indicated as a setting value.

SV Display Status Indicators


Indicates which set value is on the PV or SV display.

Unit of Measure

Attach the appropriate label showing the unit of measure (enclosed).

Escape Key

Used to select the process, maximum, or minimum value to be displayed on the PV display in RUN mode.

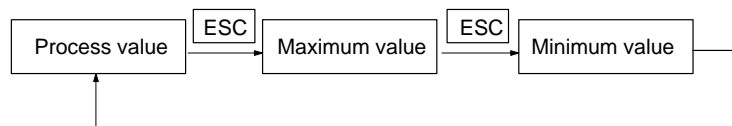


Used to return from the setting, protect, or maintenance mode to the RUN mode. This key is also used to return to the previous operation during the setting, protect, or maintenance mode.

Mode Key

Displays a setting value (out of HH, H, L, and LL setting values in this order) on the PV display in RUN mode when this key is pressed. Unless another operation key is pressed within five seconds after this key has been pressed, the display automatically changes to the one for process values.

In the RUN mode, this button terminates the measurement process and allows you to enter the setting mode, advancing through the menus and parameters.

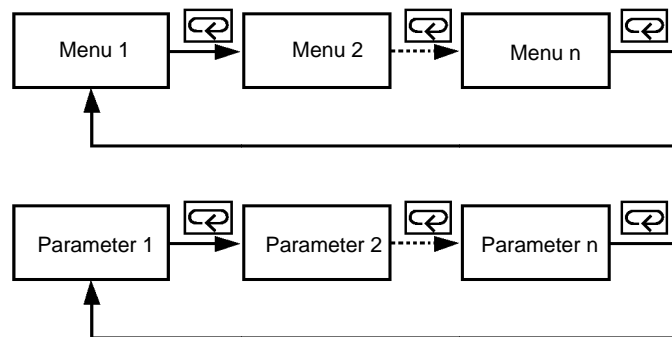


In the setting mode, this button will store changes in the non-volatile memory while at the same time advancing the display to the next menu item.

Up Key

Used to select a parameter to be displayed for setting value change.

Used to increment the current digit in the setting value by one.

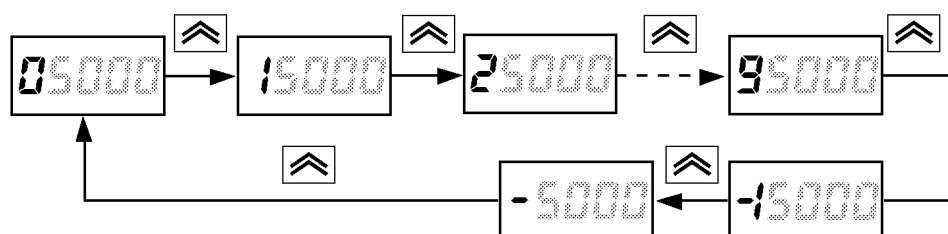

The value increases in the following order:

0, 1, 2, 3, 4, 5, 6, 7, 8, 9, (-1), and (-)

Only the leftmost digit will be displayed if the value is set to “-1” or “-.”


The value will be set to 0 if this key is pressed when “9” or “-” is displayed.

Shift Key



Used to change the parameter displayed in setting mode.

Used to scroll the digit to the right of the presently displayed digit.

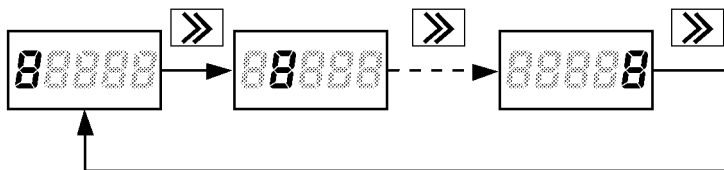

RESET/TEACH Key



Used to reset the max./min. value in RUN mode.

Used to select the teaching function. Refer to 5-1 *Teaching Function* for details.

1-3 Rear of the Meter

Terminal arrangement varies depending on the selected Output Board.


For wiring, refer to *Section 2 Setup*.

K3NH with Relay Output Board, K31-C1, -C2, -C5


K3NH with Transistor Output Board, K31-T1, -T2

K3NH with Linear Output Board, K31-L1, -L2, -L3, -L4, -L5, -L6, -L7, -L8, -L9, -L10


K3NH with RS-485 Output Board, K31-FLK2, -FLK5

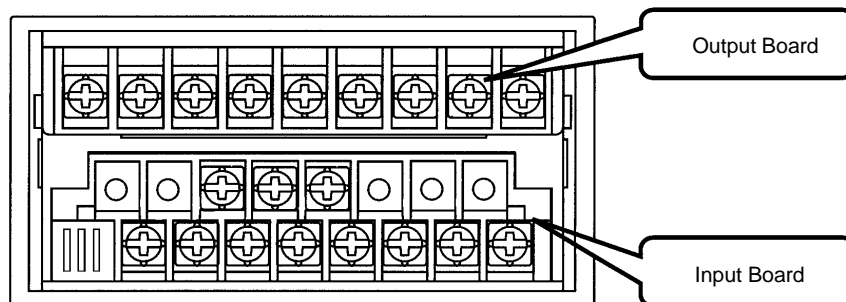


K3NH with BCD Output Board, K31-B2, -B4

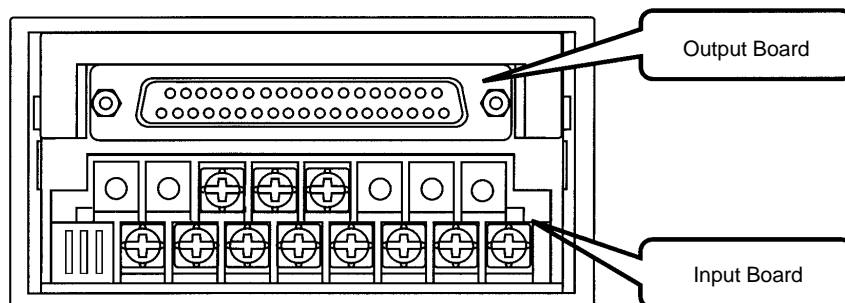


K3NH with RS-232C Output Board, K31-FLK1

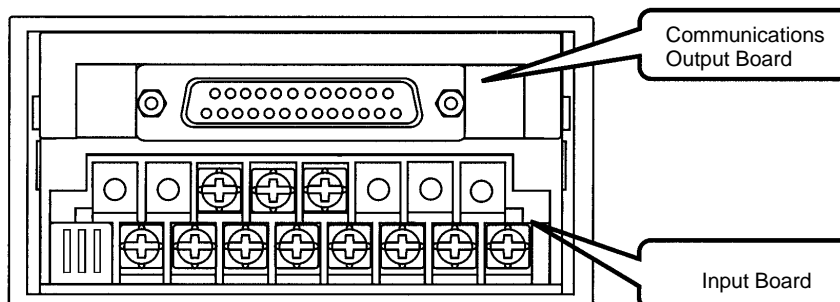

K3NH with RS-422 Output Board, K31-FLK3

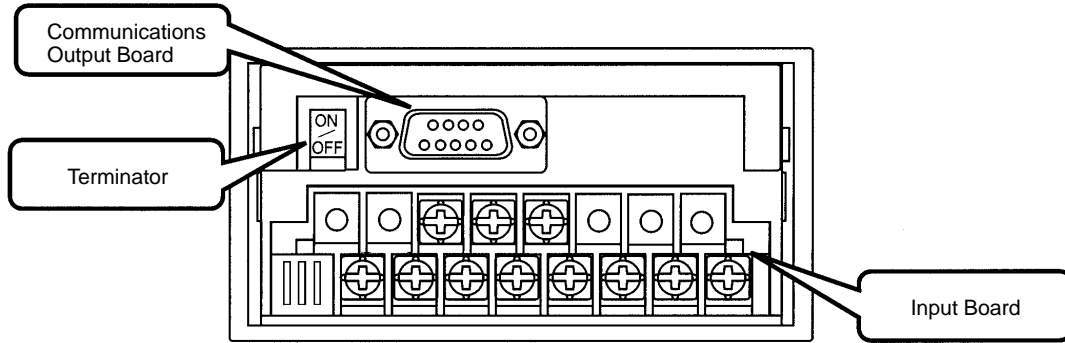

K3NH with RS232C + Transistor Output Board, K31-FLK4 K3NH with RS-422 + Transistor Output Board, K31-FLK6

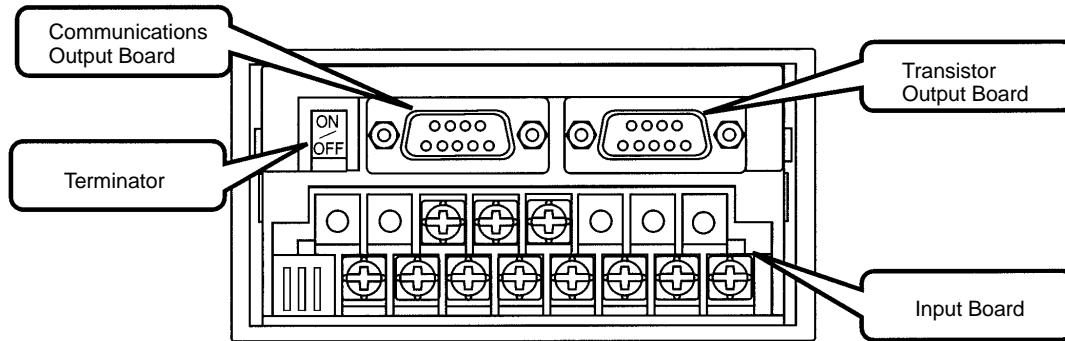


1-4 Modes

The following four modes are available.

- RUN mode for normal operations (see *Section 4 Operations in RUN Mode*)
- Setting mode for initializing parameter input (see *Section 3 Parameter Setting*)
- Protect mode for lock-out configuration (see *3-1 Protect Mode*)
- Maintenance mode for field calibration and initialization (see *5-3-3 Field Calibration* and *5-3-2 Initialization*)

Refer to the following for the relationship among these modes and selection of the modes.

Press the Mode and Shift Keys while turning on the K3NH.

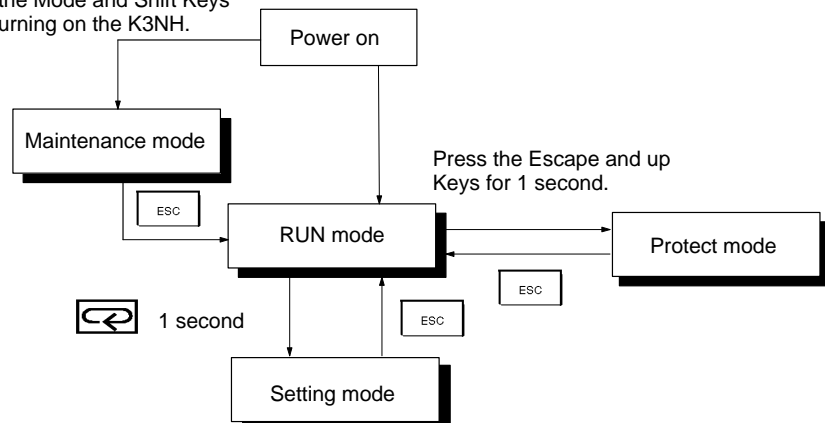

RUN Mode

K3NH is in RUN when the K3NH is turned ON.

The K3NH in this mode provides an output signal as a result of the comparison of the measured and setting values.

The basic model in this mode usually displays the process value. The maximum and minimum values are displayed by pressing the Escape Key. The parameters and setting values are displayed by pressing the Mode Key.

Refer to *Section 4 Operations in RUN Mode* for RUN mode in detail.

Setting Mode

Values are set in the K3NH in this mode by key input or using the teaching function.

Refer to *Section 3 Parameter Setting* for value setting by key input and *5-1 Teaching Function* for the teaching function in detail.

Protect Mode

Use this mode to prohibit some operations in order to lock out the setting values.

Refer to *3-1 Protect Mode* for details.

Maintenance Mode

The field calibration of the K3NH in this mode is possible. Refer to *5-3-3 Field Calibration* for details.

The setting values are reset to factory-set values in this mode. Refer to *5-3-2 Initialization* for details.

1-5 Communications Function

The communications function of the K3NH makes it possible for the host computer to perform the following operations.

- Confirmation and change of setting values. Communications conditions cannot be changed.
- Reading and resetting the maximum and minimum values.
- Forced-zero setting and resetting.
- Confirmation of model data.

Use a model with the Communications Board if the communications function is required.

Refer to the *Communications Manual* for the communications function in detail.

RS-232C

Use the K31-FLK1 or K31-FLK4 Output Board to use the RS-232C interface.

RS-422

Use the K31-FLK3 or K31-FLK6 Output Board to use the RS-422 interface.

RS-485

Use the K31-FLK2 or K31-FLK5 Output Board to use the RS-485 interface.

1-6 Field Calibration

The K3NH is correctly calibrated before shipping. Normally, therefore, the user will not need to calibrate the K3NH.

The user can calibrate the K3NH by referring to *5-3 Maintenance Mode*. OMRON does not, however, guarantee the result of calibration performed by the user.

The user should prepare calibration instruments or equipment. Before operating such instruments or equipment, be sure to read the operation manuals provided with them.

SECTION 2

Setup


This section provides instructions required for mounting and wiring the K3NH.

2-1	Mounting	10
2-2	Input Block	11
2-2-1	Terminal Arrangement	11
2-2-2	Wiring Precautions	12
2-2-3	Wiring	12
2-3	Output Board	14
2-3-1	Terminal Arrangement	14
2-3-2	Relay Output Board	16
2-3-3	Transistor and Combination Output Board	16
2-3-4	Linear Output Board	17
2-3-5	BCD Output Board	17


2-1 Mounting

Dimensions

All dimensions are in millimeters.

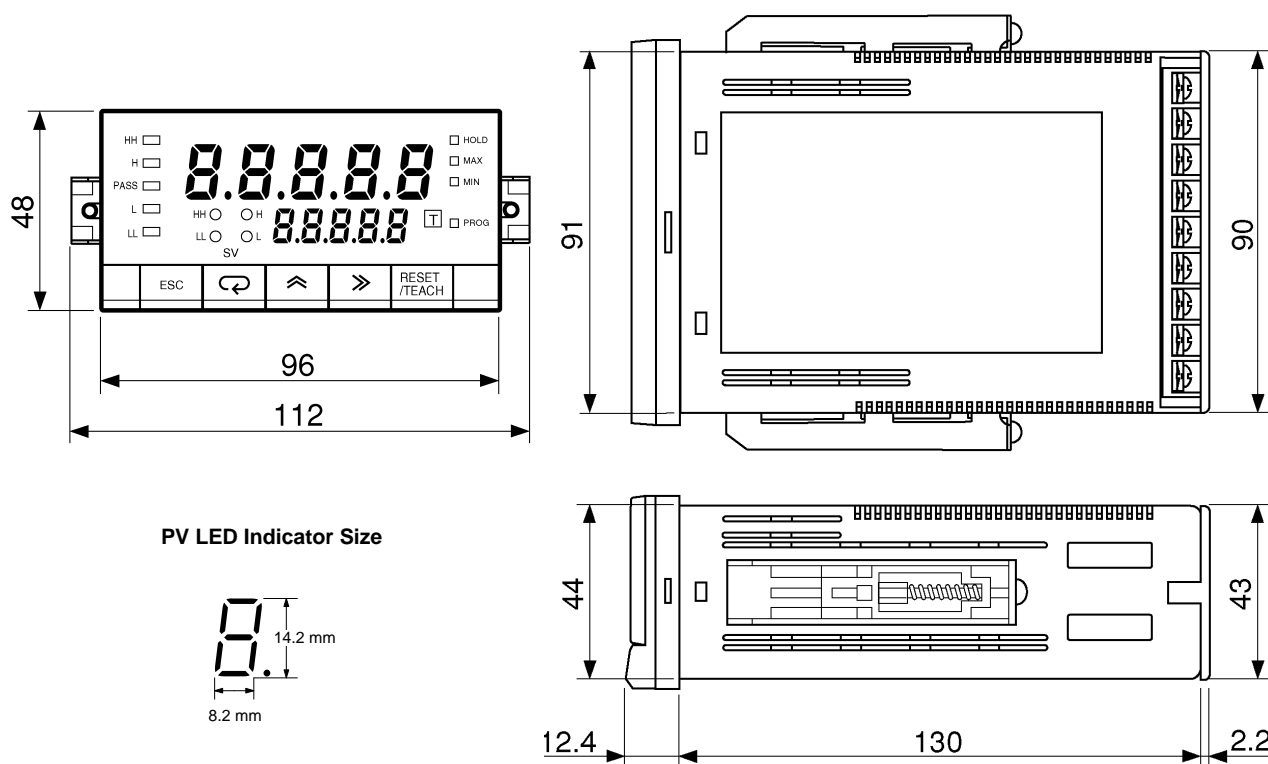


Panel Cutouts

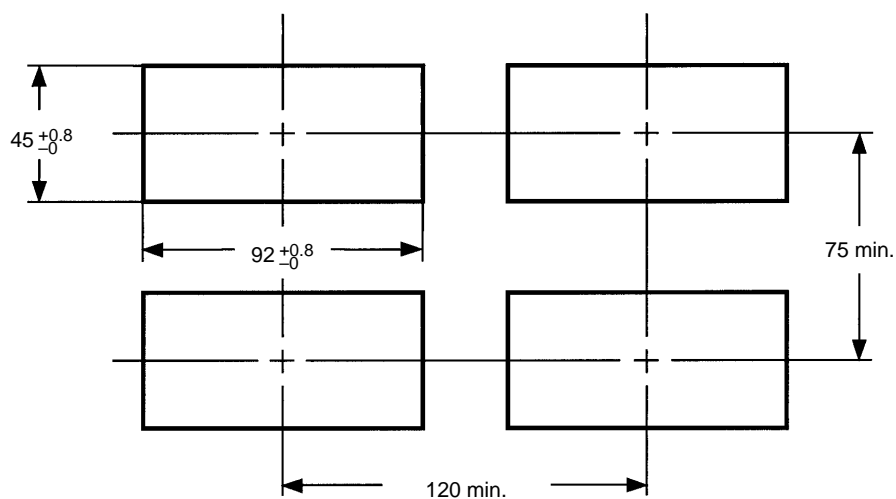

Recommended panel thickness is 1 to 3.2 mm.

Do not mount more than one Unit closely in the horizontal or vertical direction. Be sure to keep the distance between adjacent Units.


Mounting Method

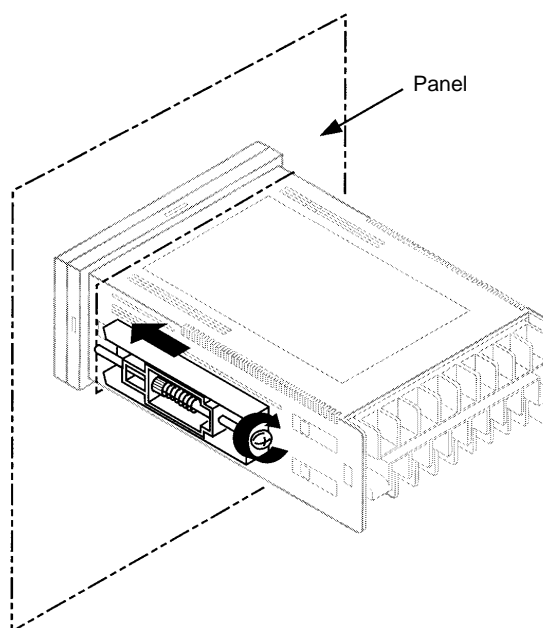

- 1, 2, 3...**
1. Insert the K3NH into the mounting hole on the panel.
 2. Hook the fixture claws onto the side holes.
 3. Mount a fixing metal to the right and left sides as shown above and while keeping them in balance, alternately tighten each screw until the ratchet becomes idle.

2-2 Input Block

2-2-1 Terminal Arrangement

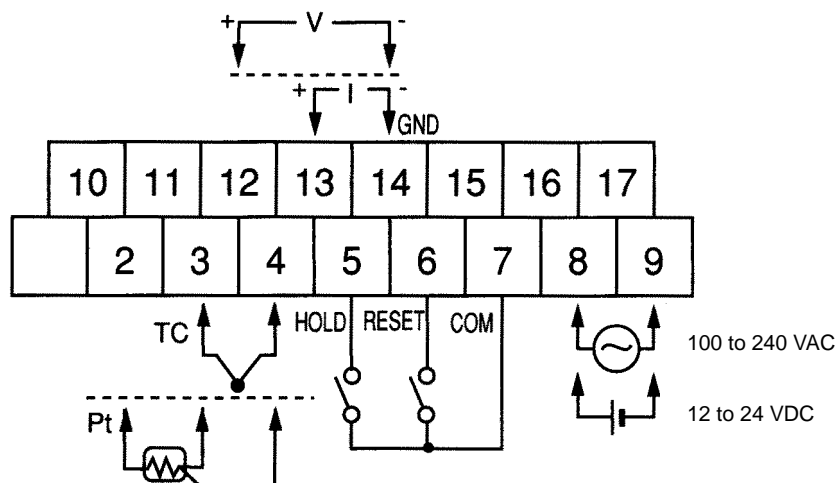

2-2-2 Wiring Precautions

- Do not make any mistake in polarity when supply DC power to the K3NH.
- Do not wire power lines alongside the signal lines of the K3NH in order to prevent against noise interference.
- Wire the terminal block with crimp terminals
- Tighten each screw to a torque of 0.78 N • m (8 kgf • cm).


2-2-3 Wiring

Power Supply

Apply 100 to 240 VAC or 12 to 24 VDC to terminals 8 and 9.

Temperature Input


Connect a platinum resistance thermometer to terminals 2, 3, and 4 or a thermocouple to terminals 3 and 4. The terminals used vary with the input type range as shown in the following table.

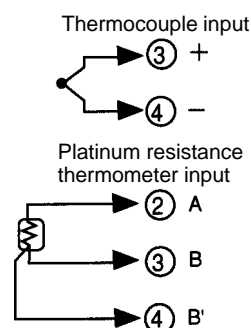

Input type	Measurement range			
	°C		°F	
	4-digit display	5-digit display	4-digit display	5-digit display
JPt100	-199.0 to 650.0	-199.0 to 650.0	-199.9 to 999.9	-199.99 to 999.99
Pt100	-199.0 to 650.0	-199.0 to 650.0	-199.9 to 999.9	-199.99 to 999.99
K1	-200 to 1,300	-200.0 to 1,300.0	-300 to 2,300	-300.0 to 2,300.0
K2	0.0 to 500.0	0.00 to 500.00	0.0 to 900.0	0.00 to 900.00
J1	-100 to 850	-100.0 to 850.0	-100 to 1,500	-100.0 to 1,500.0
J2	0.0 to 400.0	0.00 to 400.00	0.0 to 750.0	0.00 to 750.00
T	-199.9 to 400.0	-199.99 to 400.00	-199.9 to 700.0	-199.99 to 700.00
E	0 to 600	0.0 to 600.0	0 to 1,100	0.0 to 1,100.0
L1	-100 to 850	-100.0 to 850.0	-100 to 1,500	-100.0 to 1,500.0
L2	0.0 to 400.0	0.00 to 400.00	0.0 to 750.0	0.00 to 750.00
U	-199.9 to 400.0	-199.99 to 400.00	-199.9 to 700.0	-199.99 to 700.00
N	-200 to 1,300	-200.0 to 1,300.0	-300 to 2,300	-300.0 to 2,300.0
R	0 to 1,700	0.0 to 1,700.0	0 to 3,000	0.0 to 3,000.0
S	0 to 1,700	0.0 to 1,700.0	0 to 3,000	0.0 to 3,000.0
B	100 to 1,800	100.0 to 1,800.0	300 to 3,200	300.0 to 3,200.0
W	0 to 2,300	0.0 to 2,300.0	0 to 4,100	0.0 to 4,100.0
PLII	0 to 1,300	0.0 to 1,300.0	0 to 2,300	0.0 to 2,300.0

Voltage/Current Input

Connect sensor output to terminals 12 through 14.

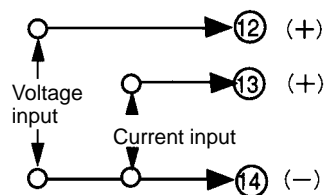


Connect a sensor with an output of 0 to 5 V, 1 to 5 V, or 0 to 10 V to terminals 12 through 14.

Connect a sensor with an output of 0 to 20 mA or 4 to 20 mA to terminals 13 and 14.

Input type	Input range	Default display range
DC current	4 to 20 mA	0 to 100
	0 to 20 mA	0 to 100
DC voltage	1 to 5 V	0 to 100
	0 to 5 V	0 to 100
	0 to 10 V	0 to 100

External Control Input**HOLD Input****RESET Input**

Connect external signal input to terminals 5 to 7.

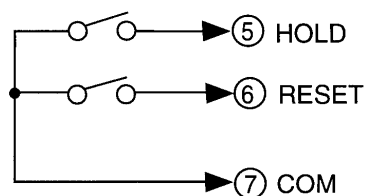

Connect hold signal (HOLD) input to terminal 5.

Connect reset signal (RESET) input to terminal 6.

The transistor satisfying the following conditions must be used to input open collector external signals.

- Residual voltage with transistor turned on: 3 V max.
- Current leakage with transistor turned off: 1.5 mA max.

Approximately 5 V is imposed between COM and terminals 5 and 6 with a current flow of approximately 18 mA (a nominal value) at the time of external input short-circuiting.

2-3 Output Board


2-3-1 Terminal Arrangement

K3NH with Relay Output Board, K31-C1, -C2, -C5


K3NH with Transistor Output Board, K31-T1, -T2

K3NH with Linear Output Board, K31-L1, -L2, -L3, -L4, -L5, -L6, -L7, -L8, -L9, -L10


K3NH with RS-485 Output Board, K31-FLK2, -FLK5

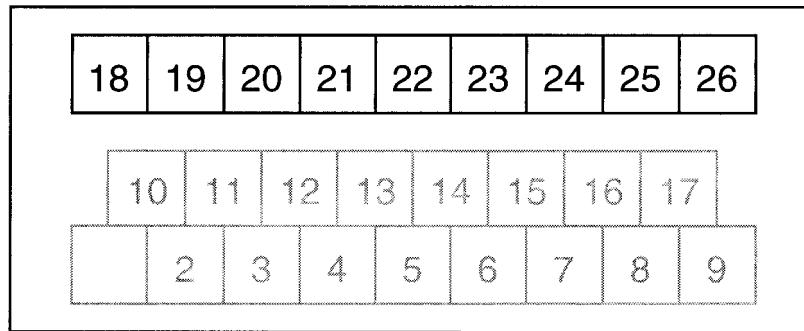


K3NH with BCD Output Board, K31-B2, -B4

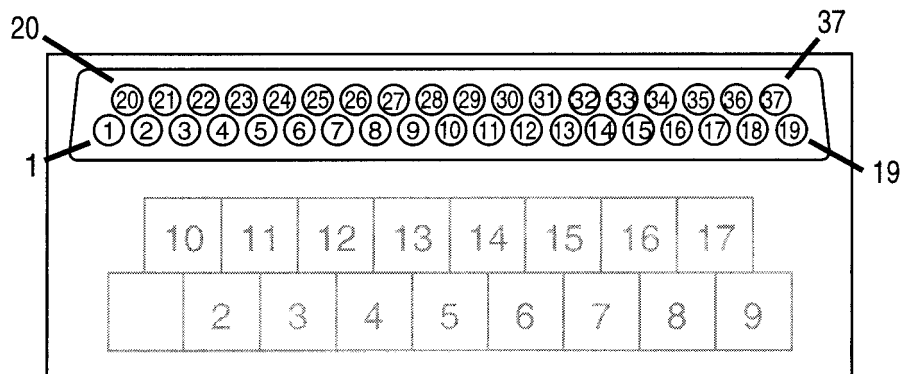


K3NH with RS-232C + Transistor Output Board, K31-FLK4

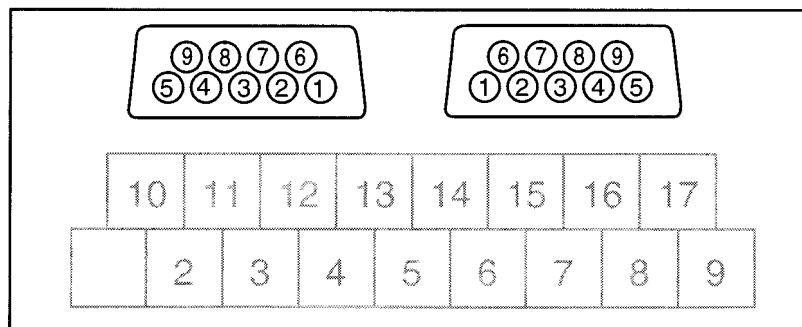


K3NH with RS-422 + Transistor Output Board, K31-FLK6

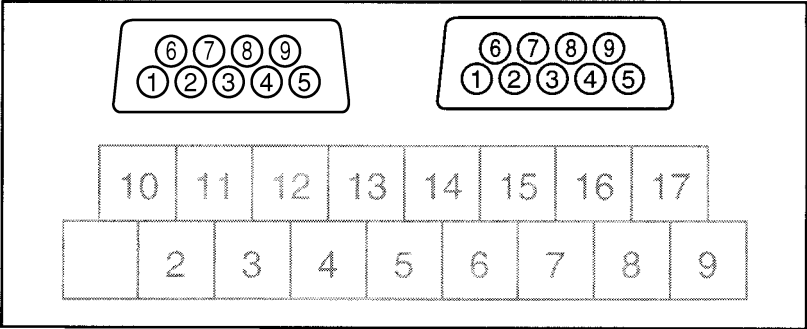

K3NH with RS-232C Output Board, K31-FLK1

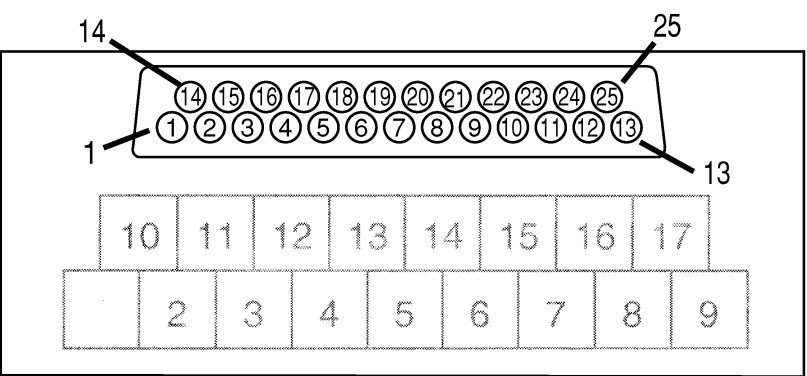


K3NH with RS-422 Output Board, K31-FLK3

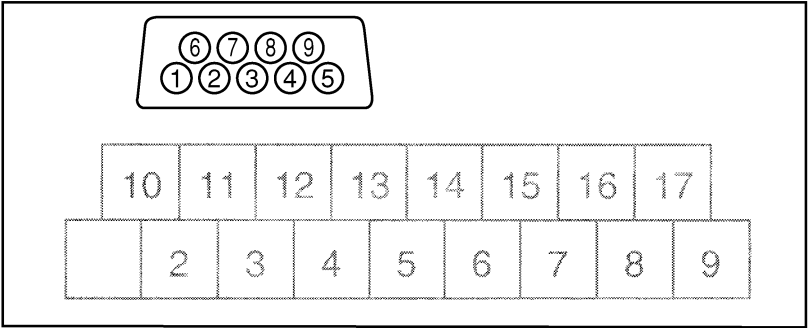


2-3-2 Relay Output Board

The following figures show the connections for relay output.

K3NH with 3 Relay Output Boards, K31-C1

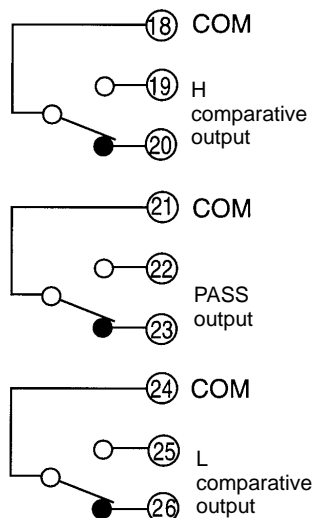

K3NH with 5 Relay Output Boards, K31-C2

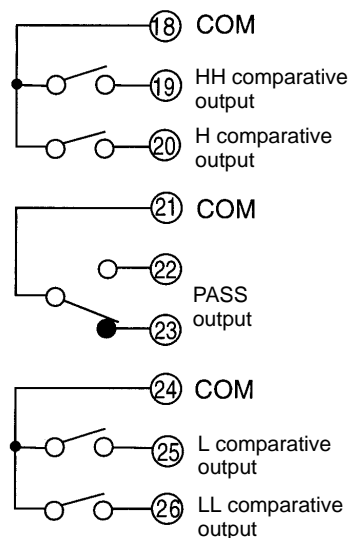

The following contact output conditions are required.

- 5 A (resistive load) at 250 VAC
- 1.5 A (inductive load) at 250 VAC
- 5 A (resistive load) at 30 VDC
- 1.5 A (inductive load) at 30 VDC

2-3-3 Transistor and Combination Output Board

K3NH with Transistor Output Board, K31-T1 or K31-T2




K3NH with Linear Output Board, K31-L4, -L5, -L6, -L9, -L10

K3NH with RS-485 + 5 Relay Output Boards, K31-FLK5

K3NH with BCD Output Board, K31-B2 or K31-B4

K3NH with RS232C + 5 Transistor Output Boards, K31-FLK4

K3NH with RS-422 + 5 Transistor Output Boards, K31-FLK6

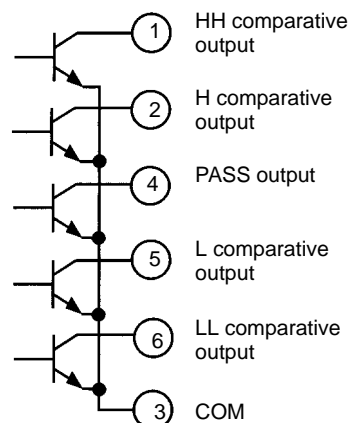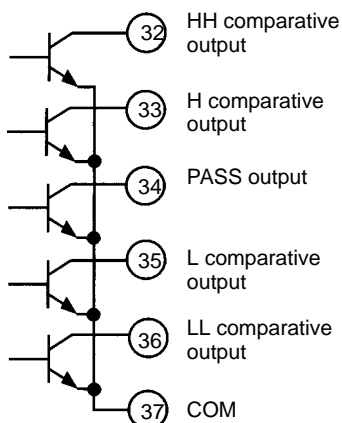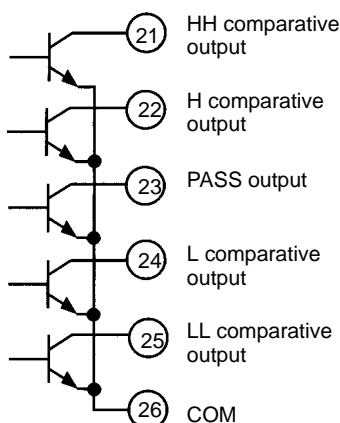

The following transistor output conditions are required.


Maximum rated voltage: 24 VDC

Load current: 50 mA

Current leakage with transistor turned off: 100 μ A.

2-3-4 Linear Output Board

The following figures show connections for linear output.

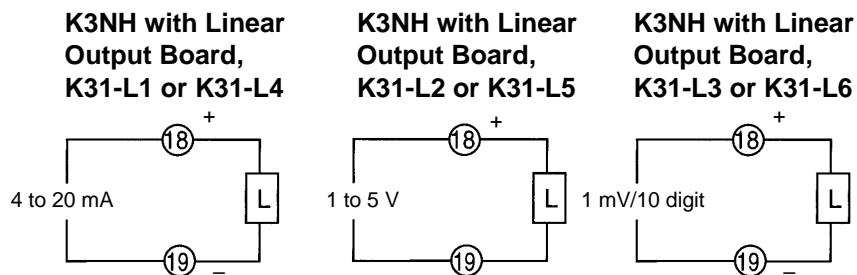

The following linear output conditions are required.

Linear output	Permissible load resistance	Resolution	Output error
4 to 20 mA	600 Ω max.	4096	$\pm 0.5\%$ FS
1 to 5 V	500 Ω min.	4096	$\pm 0.5\%$ FS
1 mV/10 digit	1 k Ω min.	4096	$\pm 1.5\%$ FS

2-3-5 BCD Output Board

Refer to *Section 6 BCD Output* for the terminal arrangement and interface.

SECTION 3

Parameter Setting

This section provides instructions for setting the parameters of the K3NH with key inputs. Be sure to read this section before using the K3NH Temperature Meter for the first time.

3-1	Overview	20
3-1-1	Heading Symbols	20
3-1-2	Setting Procedures	20
3-2	Setting Mode	21
3-2-1	Selecting Setting Mode	21
3-2-2	Menu Overview	22
3-2-3	Setting Value Menu (5u5Et)	23
	HH Set Value (5u.HH)	23
	H Set Value (5u. H)	23
	L Set Value (5u. L)	23
	LL Set Value (5u.LL)	23
3-2-4	Setup Menu (SEtUP)	27
	Input Type (Ln-t)	27
	Temperature Unit (C-F)	29
	Scaling Upper Limit Value (Ln-H)	31
	Scaling Lower Limit Value (Ln-L)	31
	Decimal Point Position (dEL-P)	31
	Communications Unit Number (U-nā)	34
	Baud Rate (bPS)	34
	Word Length (LEn)	36
	Stop Bits (5bL-t)	36
	Parity Bits (Pr-tY)	36
3-2-5	Option Menu (ōP-t)	39
	Average Processing (AuG)	39
	Display Digit Change (dL-tL-t)	42
	Upper-limit Compensation Value (Ln5H)	44
	Lower-limit Compensation Value (Ln5L)	44
	Hysteresis (HY5)	46
	Comparative Output Pattern (C-ōU-t)	48
	Standby Sequence (5tdbY)	51
	Upper Limit (H) of Linear Output Range (L5Et.H)	53
	Lower Limit (L) of Linear Output Range (L5Et.L)	53
	Remote/Local Programming (r-L)	56
3-3	Protect Mode	58
3-3-1	Selecting Protect Mode	58
3-3-2	Menu Overview	59
3-3-3	Protect Menu (Pr-ō-t)	60
	All Key Protect (ALL)	60
	Setting Value Change Prohibit (5u5Et)	61
	Maximum/Minimum Value Clear Prohibit (āā.r5-t)	63
	Security (5EL-r)	65

3-1 Overview

3-1-1 Heading Symbols

The following symbols are used for headings in this section.



FUNCTION

This symbol precedes an explanation of the parameter's meaning and function.



SETTING

This symbol precedes a description of the settings, setting range, and default value.



PROCEDURE

This symbol precedes an explanation of procedures for parameters that specify operations.



REFERENCE

This symbol precedes a listing of references and related parameters.



MODELS

This symbol precedes a listing of the models in which this parameter can be used.

3-1-2 Setting Procedures

- The K3NH has four modes: RUN mode for normal operations, Setting mode for initial parameter input, Protect mode for lock-out configuration, and Maintenance mode for initializing set values and user calibration. The parameters that are accessible on any individual K3NH will vary depending on the Output Board installed. Refer to *Appendix D Available Parameters*.
- The K3NH is in RUN mode when the K3NH is turned on. Parameter settings in protect or setting mode are described below on the basis that the parameters are set for the first time.

For the operation in RUN mode, refer to *Section 4 Operations in RUN Mode*.


- The setting examples are provided on condition that the factory-set values of the K3NH have not been changed.

3-2 Setting Mode

3-2-1 Selecting Setting Mode

- The K3NH in RUN mode will go into setting mode if the Mode Key is pressed for 1 s minimum.
- The K3NH in setting mode will go into RUN mode if the Escape Key is pressed.


Press the Mode and Shift Keys while turning the K3NH on.

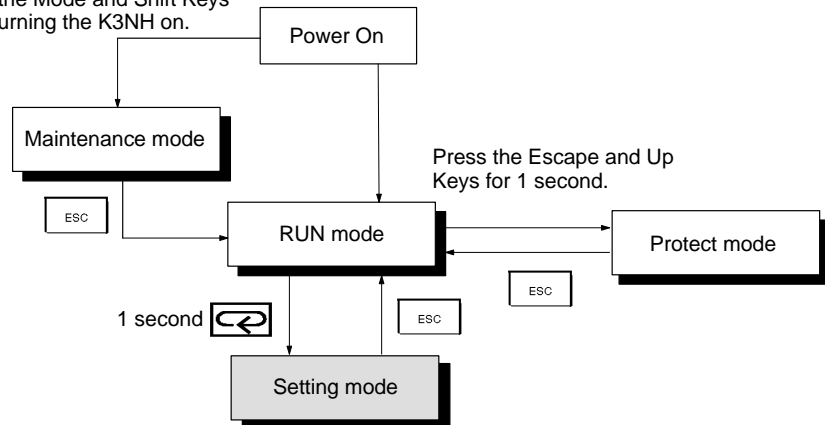





- The menu in each mode changes whenever the Mode Key is pressed.
- If the Mode Key is pressed for more than one second while a menu is displayed, a parameter will be displayed.
- The parameter changes whenever the Mode Key is pressed.
- If the Shift Key is pressed while a parameter is displayed, the parameter will be ready to change.
- Press the Up Key to change parameters.
- The digit of a set value is selected with the Shift Key and changed with the Up Key.
- The PROG indicator is lit while a menu or parameter is displayed.
- The PROG indicator flashes during a set value change.


Note If the input type is changed, all the other parameters will be set to default values. Therefore, set the input type first.

3-2-2 Menu Overview

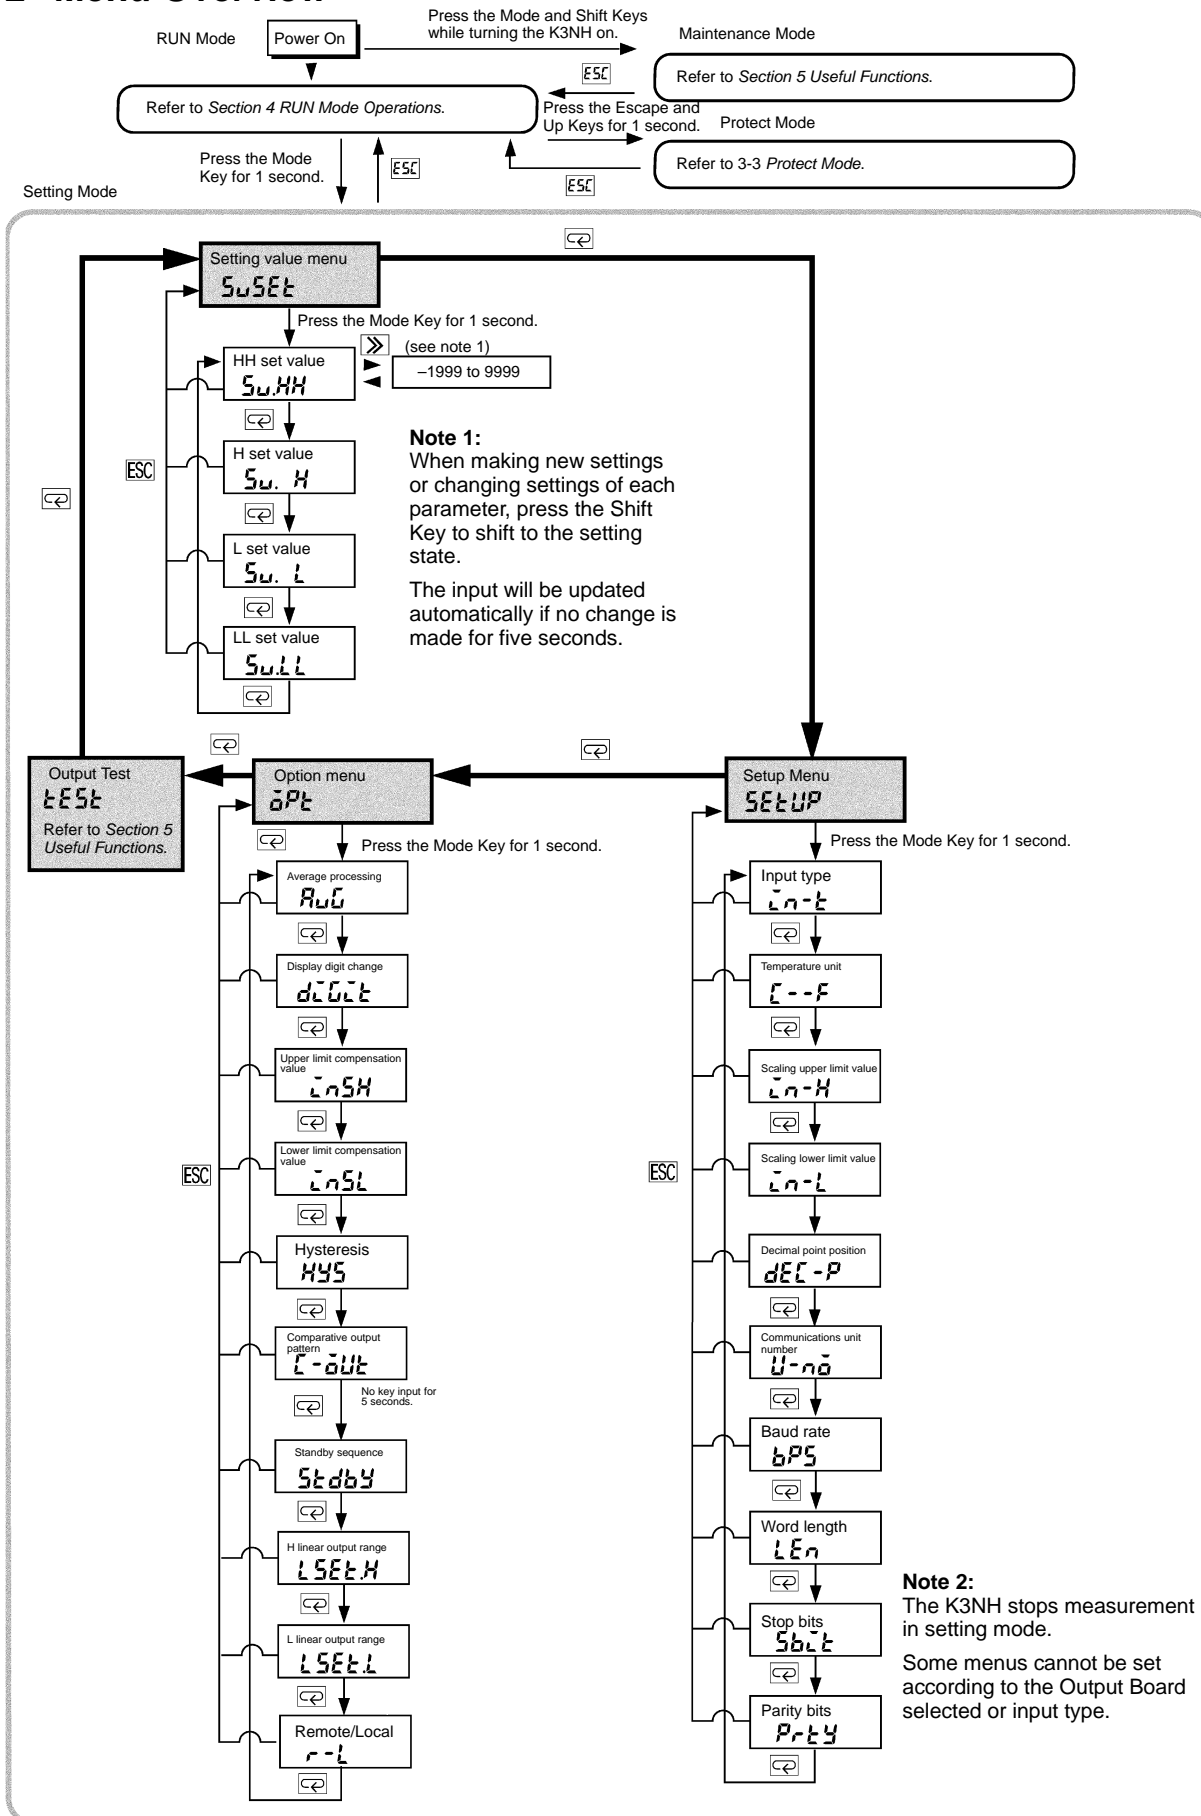

3-2-3 Setting Value Menu (*SVSET*)


	<u>HH Set Value</u>
	<u>H Set Value</u>
	<u>L Set Value</u>
	<u>LL Set Value</u>



FUNCTION



SETTING



REFERENCE



MODELS

- There are two basic methods for setting HH, H, L, and LL set values: by entering during RUN mode via the front-panel buttons, setting in Setting mode, or by the teaching function.

Setting	Setting range	Default
HH set value	–1999 to 9999	9999
H set value	–1999 to 9999	9999
L set value	–1999 to 9999	–1999
LL set value	–1999 to 9999	–1999

Refer to 5-1 *Teaching Function*.

Refer to 4-1 *Displaying and Changing Set Values*.

- The setting value menu is only available for K3NH with Comparative Output Board.

SETTING
EXAMPLE

Follow the steps described below to input the following.

Setting value HH = "400"



Setting value H = "300"

Setting value L = "200"

Setting value LL = "100"

Set Value LED Display Model



Basic Model



- 1, 2, 3... 1. Press the Mode Key for more than one second while the *SuSEt* setting value menu is displayed. The *Su.HH* HH setting value setting will be displayed.

Set Value LED Display Model


Basic Model



2. Press the Shift Key to display the set value *9999* for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model




3. Press the Up and Shift Keys to set the value to *400*. The input will be validated automatically if no change is made for five seconds. The *Su.HH* HH setting value setting will be displayed again.

Note Press the Mode Key to enter the set value immediately. The *Su.H* H setting value setting will be displayed for setting the next parameter.

Set Value LED Display Model



Basic Model



4. Press the Mode Key to display the *Su.H* H setting value setting.

Set Value LED Display Model


Basic Model



5. Press the Shift Key to display the set value *9999* for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model



6. Press the Up and Shift Keys to set the value to *300*. The input will be validated automatically if no change is made for five seconds. The *Su. H H* setting value setting will be displayed again.


Note Press the Mode Key to enter the set value immediately. The *Su. L L* setting value setting will be displayed for setting the next parameter.

Set Value LED Display Model Basic Model




7. Press the Mode Key to display the *Su. L L* setting value setting.

Set Value LED Display Model Basic Model



8. Press the Shift Key to display the set value *-1999* for changing. The PROG indicator will flash.

Set Value LED Display Model Basic Model



9. Press the Up and Shift Keys to set the value to *200*. The input will be validated automatically if no change is made for five seconds. The *Su. L L* setting value setting will be displayed again.


Note Press the Mode Key to enter the set value immediately. The *Su.LL LL* setting value setting will be displayed for setting the next parameter.

Set Value LED Display Model Basic Model



10. Press the Mode Key to display the *Su.LL LL* setting value setting.

Set Value LED Display Model Basic Model



11. Press the Shift Key to display the set value *-1999* for changing. The PROG indicator will flash.

Set Value LED Display Model Basic Model




12. Press the Up and Shift Keys to set the value to 100 . The input will be validated automatically if no change is made for five seconds. The $S_{u.LL}$ LL setting value setting will be displayed again.

Note Press the Mode Key to enter the set value immediately. The $S_{u.HH}$ HH setting value setting will be displayed for setting the next parameter.

Set Value LED Display Model



Basic Model




13. Press the Mode Key to display the $S_{u.HH}$ HH set value setting.

Set Value LED Display Model

Basic Model



3-2-4 Setup Menu (SETUP)



Input Type



FUNCTION




SETTING

The following table lists the types of thermocouples, temperature-resistance thermometers, voltage, and current available to the K3NH.

Default Settings: K1

Input type	Setting	Input type	Setting
JPt100	JPt	N	n
Pt100	Pt	R	r Pr
K1	K1 CR	S	S Pr
K2	K2 CR	B	b Pr
J1	J1 CC	W	W26
J2	J2 CC	PLII	PL 2
T	t CC	4 to 20 mA	4-20
E	E Cr	0 to 20 mA	0-20
L1	L1 CC	1 to 5 V	1-5
L2	L2 CC	0 to 5 V	0-5
U	U CC	0 to 10 V	0-10



REFERENCE

Refer to 2-2 Input Block.

SETTING
EXAMPLE

Follow the steps described below to set the input type to J2 CC.

Set Value LED Display Model

Basic Model





1, 2, 3...

1. Press the Mode Key for more than one second while the *SETUP* setup menu is displayed. The *L1-L2* input range setting will appear.

Set Value LED Display Model



Basic Model



2. Press the Shift Key to display the present set value *P1 CR* for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model




3. Repeatedly press the Up Key until $\overline{2} \overline{2} \overline{2}$ is displayed. The displayed setting will be validated automatically if no change is made for five seconds. The $\overline{2} \overline{2} \overline{2}$ input range setting will be displayed again.

Set Value LED Display Model	Basic Model
------------------------------------	--------------------


When no operation is executed for five seconds

Set Value LED Display Model Basic Model

Note Press the Mode Key to enter the displayed setting immediately. The next parameter will be displayed for setting.



Temperature Unit



FUNCTION



SETTING

The following menu settings determine the unit of measured temperature.

Setting	Default
C: °C	C
F: °F	

SETTING EXAMPLE

Follow the steps described below to set the temperature unit to °F.

Set Value LED Display Model



Basic Model



- 1, 2, 3... 1. Press the Mode Key for more than one second while the *SETUP* setup menu is displayed. The *C-F* input type setting will appear.

Set Value LED Display Model



Basic Model



2. Press the Mode Key to display *C-F* temperature unit menu.

Set Value LED Display Model



Basic Model



3. Press the Shift Key to display the present set value *C* for changing. The PROG indicator will flash.

Set Value LED Display Model



Basic Model



4. Press the Up Key to display *F*. The displayed setting will be validated automatically if no change is made for five seconds. The *C-F* input type setting will be displayed again.


Set Value LED Display Model

Basic Model




When no operation is executed for five seconds

Set Value LED Display Model



Basic Model



Note Press the Mode Key to enter the displayed setting immediately. The next parameter will be displayed for setting.

Ln-H

Scaling Upper Limit Value

Ln-L

Scaling Lower Limit Value


dec-P

Decimal Point Position

FUNCTION


In the case of voltage or current inputs, by setting input value 1 to correspond to the scaling lower limit value and input value 2 to correspond to scaling upper limit value, scaling can be displayed for the line that connects these input values together.

Scaling values are displayed only for voltage or current inputs. Scaling values cannot be displayed for thermocouple or temperature-resistance thermometer inputs.

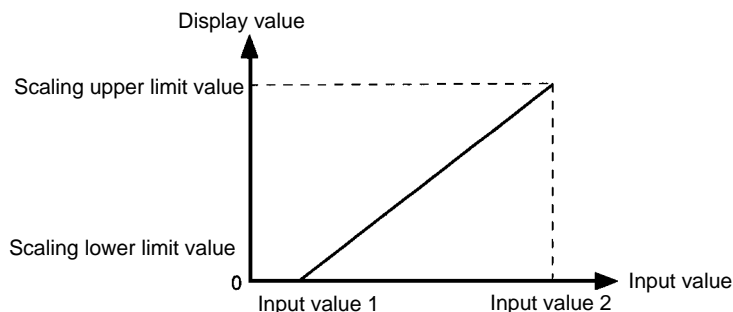**Scaling**

Sensor voltage or current output is converted into a value within a specified range.

For example, if a sensor with 4- to 20-mA output is connected to the K3NH and the K3NH is set so that it will display "0" for 4-mA input and "999" for 20-mA input, the following will be the relationship between input and display values.

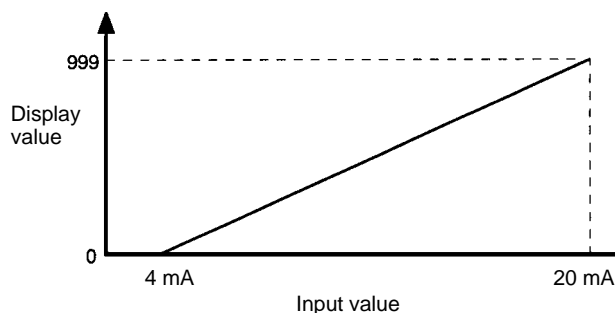

SETTING

• Scaling Value

Setting	Setting range	Default value
Scaling upper limit value	-1999 to 9,999	100
Scaling lower limit value	-1999 to 9,999	0

• Decimal Point Position

Setting range	Default value
0000 000.0 00.00 0.000	0000



REFERENCE

Refer to 5-1 Teaching Function.

SETTING
EXAMPLE

Follow the steps described below to input the following.

Scaling upper limit value = "500"

Scaling lower limit value = "100"

Decimal point position = "000.0"

Set Value LED Display Model



Basic Model



- 1, 2, 3... 1. Press the Mode Key for more than one second while the *SETUP* setup menu is displayed. The *n-L* input type setting will appear.

Set Value LED Display Model



Basic Model



2. Press the Mode Key twice to display *n-H* scaling upper limit value setting.

Set Value LED Display Model


Basic Model



3. Press the Shift Key to display the present set value *100* for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model




4. Press the Up and Shift Keys to set the value to *500*. The input value will be validated automatically if no change is made for five seconds. The *n-H* scaling upper limit value setting will be displayed again.

Note Press the Mode Key to enter the set value immediately. The *n-L* scaling lower limit value setting will be displayed for setting the next parameter.

Set Value LED Display Model


Basic Model



5. Press the Mode Key to display *n-L* scaling lower limit value setting.


Set Value LED Display Model

Basic Model



6. Press the Shift Key to display the present set value 000 for changing. The PROG indicator will flash.

Set Value LED Display Model Basic Model



7. Press the Up and Shift Keys to set the value to 100 . The input value will be validated automatically if no change is made for five seconds. The $Ln-L$ scaling lower limit value setting will be displayed again.

Note Press the Mode Key to enter the set value immediately. The $dEC-P$ decimal point position setting will be displayed for setting the next parameter.

Set Value LED Display Model Basic Model



8. Press the Mode Key to display $dEC-P$ decimal point position setting.

Set Value LED Display Model Basic Model



9. Press the Shift Key to display the present set value 0000 for changing. The PROG indicator will flash.


Set Value LED Display Model Basic Model



10. Press the Shift Key to set the value to 000.0 . The input value will be validated automatically if no change is made for five seconds. The $dEC-P$ decimal point position setting will be displayed again.

Note Press the Mode Key to enter the set value immediately. The next parameter will be displayed for setting.

Set Value LED Display Model Basic Model



When no operation is executed for five seconds

Set Value LED Display Model Basic Model



U-nō

Communications Unit Number


bPS

Baud Rate

FUNCTION



SETTING



MODELS

- Set a communications unit number as an identification number by which the host computer is connected to the K3NH.
- If more than one K3NH is connected in parallel, make sure that each communications unit number is unique.
- The baud rate should be set to the baud rate of the host computer.

- Communications Unit Number

Setting range	Unit	Default
00 to 99	---	00

- Baud Rate

Setting range	Default
1200: 1,200 bps / 2400: 2,400 bps / 4800: 4,800 bps / 9600: 9,600 bps / 19200: 19.2 Kbps / 38400: 38.4 Kbps	9600

This setting is available for the K3NH with the Communications Output Board.

SETTING EXAMPLE



Follow the steps described below to set the communications unit number to 15 and the baud rate to 19,200 bps.

Set Value LED Display Model**Basic Model**

- 1, 2, 3...
1. Press the Mode Key for more than one second while the *SETUP* setup menu is displayed. The *U-nō* input range setting will appear.

Set Value LED Display Model**Basic Model**

2. Repeatedly press the Mode Key until the *U-nō* communications unit number setting is displayed.

Set Value LED Display Model**Basic Model**

3. Press the Shift Key to display the prior set value 00 for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model




4. Press the Up and Shift Keys to set the value to 15 . The input value will be validated automatically if no change is made for five seconds. The $U-n0$ communications unit number setting will be displayed again.

Note Press the Mode Key to enter the set value immediately. The next parameter will be displayed for setting.

Set Value LED Display Model


Basic Model



5. Press the Mode Key to display the $6P5$ baud rate setting.

Set Value LED Display Model


Basic Model



6. Press the Shift Key to display the prior set value 9600 for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model



7. Press the Up Key to set the value to 19200 . The input will be validated automatically if no change is made for five seconds. The $6P5$ baud rate setting will be displayed again.

Note Press the Mode Key to enter the set value immediately. The next parameter will be displayed again for setting.

Set Value LED Display Model



Basic Model





8. Press the Up Key to enter the set value for setting the next parameter. The input value will be validated automatically if no change is made for five seconds. The $6P5$ baud rate setting will be displayed again.

Set Value LED Display Model

Basic Model



**Word Length****Stop Bits****Parity Bits**

FUNCTION



SETTING

- The communications format used for communicating with the host computer is set in the setup menu.
- Refer to the *Communications Manual* for the communications format in detail.

- Word Length

Setting	Unit	Default
7/8	bit	7


- Stop Bits

Setting	Unit	Default
1/2	bit	2

- Parity Bit

Setting	Default
$\bar{n}\bar{o}\bar{n}\bar{E}$: None $E\bar{u}\bar{E}\bar{n}$: Even $\bar{o}\bar{d}\bar{d}$: Odd	$E\bar{u}\bar{E}\bar{n}$

This setting is available for the K3NH with the Communications Output Board.



MODELS

**SETTING
EXAMPLE**

Follow the steps described below to set the following.


Word length: 8 bits

Number of stop bits: 1



Parity bits: $\bar{n}\bar{o}\bar{n}\bar{E}$

Set Value LED Display Model**Basic Model**

- 1, 2, 3... 1. Press the Mode Key for more than one second while the *SETUP* setup menu is displayed. The $\bar{n}\bar{o}\bar{n}\bar{E}$ input range setting will appear.


Set Value LED Display Model**Basic Model**

2. Repeatedly press the Mode Key until the *LEn* word length setting is displayed.


Set Value LED Display Model**Basic Model**

3. Press the Shift Key to display the prior set value 7 for changing. The PROG indicator will flash.

Set Value LED Display Model




Basic Model




4. Press the Up Key to set the value to 8. The input value will be validated automatically if no change is made for five seconds. The LEN word length setting will be displayed again.

Note Press the Mode Key to enter the set value immediately. The next parameter will be displayed for setting.

Set Value LED Display Model




Basic Model




5. Press the Mode Key to display the 5bit stop bit setting.

Set Value LED Display Model



Basic Model




6. Press the Shift Key to display the set value 2 for changing.

Set Value LED Display Model




Basic Model




7. Press the Up Key to set the value to 1. The input will be validated automatically if no change is made for five seconds. The 5bit stop bit setting will be displayed again.

Note Press the Mode Key to enter the set value immediately. The next parameter will be displayed for setting.

Set Value LED Display Model



Basic Model




8. Press the Mode Key to display the Prty parity bit setting.

Set Value LED Display Model




Basic Model




9. Press the Shift Key to display Even for changing.

Set Value LED Display Model




Basic Model




10. Press the Up Key to display $n\bar{o}nE$. The setting will be validated automatically if no change is made for five seconds. The P_rEY parity bit setting will be displayed again.

Note Press the Mode Key to enter the setting immediately. The next parameter will be displayed for setting.

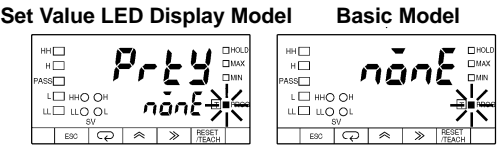


When no operation is executed for five seconds

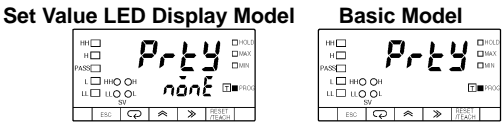

3-2-5 Option Menu (\bar{OPT})

AUG

Average Processing

FUNCTION





SETTING




REFERENCE

- The average processing of inputs are enabled for setting.
- Average processing prevents the display from fluctuating due to unstable input.
- Select simple average processing or movement average processing and the number of sampling times.

Setting	Default
1: No average processing	1
00002: Movement average processing by sampling 2 times	
00004: Movement average processing by sampling 4 times	
00008: Movement average processing by sampling 8 times	
00016: Movement average processing by sampling 16 times	
50002: Simple average processing by sampling 2 times	
50004: Simple average processing by sampling 4 times	
50008: Simple average processing by sampling 8 times	
50016: Simple average processing by sampling 16 times	

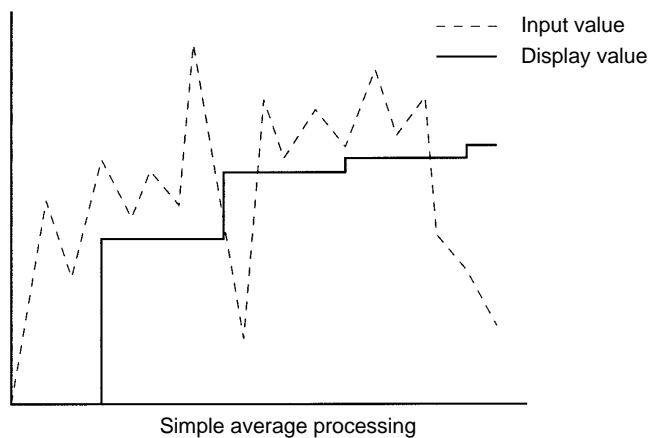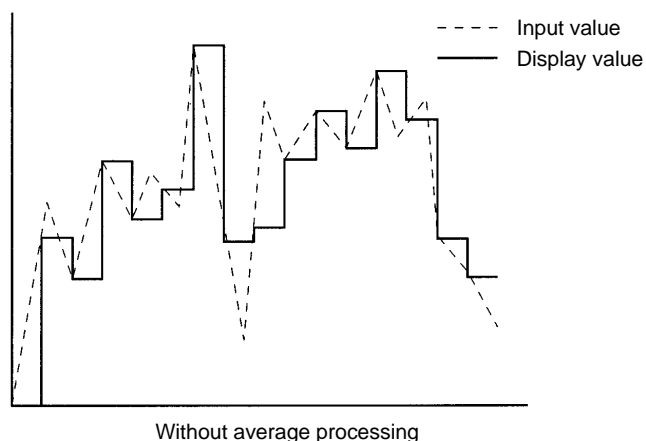

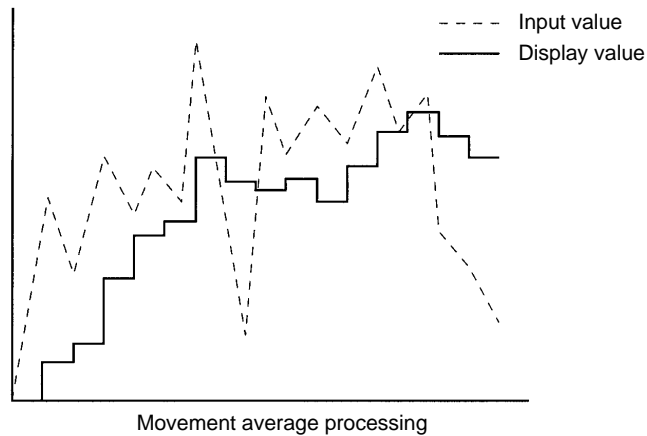**Simple Average Processing:**

The average value is displayed after the input is sampled “n” times.

The previous value is displayed until the sampling is complete.

Simple average processing is ideal for a display refresh period that is comparatively long.

The number of sampling times can be set to 2, 8, 16, or 32.

Movement Average Processing


When an input is sampled, the new sampling data is added to the previous sampling data and averaged.

Movement average processing is ideal for removing cyclic noise from the input signal.



The number of sampling times can be set to 2, 8, 16, or 32.

**SETTING
EXAMPLE**



Follow the steps described below to set the number of movement average processing times to 16.

Set Value LED Display Model**Basic Model**

- 1, 2, 3...** 1. Press the Mode Key for more than one second while the $\bar{d}Pt$ option menu is displayed. The AvG average processing setting will appear.


Set Value LED Display Model**Basic Model**

2. Press the Shift Key to display the prior setting \bar{I} for changing. The PROG indicator will flash.


Set Value LED Display Model**Basic Model**


3. Repeatedly press the Up Key until $\overline{A00\ 16}$ is displayed. The setting will be validated automatically if no change is made for five seconds. The \overline{AUG} average processing setting will be displayed again.

Note Press the Mode Key to enter the set value immediately. The next parameter will be displayed for setting.

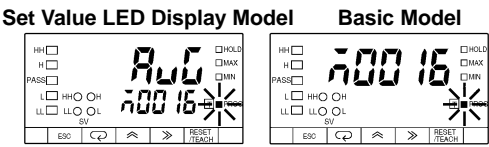


When no operation is executed for five seconds

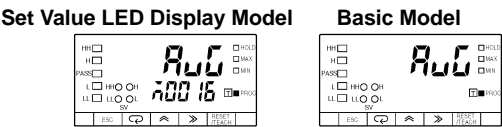



Display Digit Change



FUNCTION



SETTING

- The number of digits of data displayed by the K3NH is set in the option menu.
- A maximum of four digits can be set regardless of the number of actual digits.


Setting range	Unit	Default
4/5	---	4

SETTING EXAMPLE

Follow the steps described below to set the displayed number of digits to five.

Set Value LED Display Model

Basic Model




1, 2, 3...

1. Press the Mode Key for more than one second while the *dPt* option menu is displayed. The *Avg* average processing setting will appear.

Set Value LED Display Model



Basic Model



2. Press the Mode Key to display the *d.c.c.t* display digit change setting.

Set Value LED Display Model



Basic Model



3. Press the Shift Key to display present set value 4 for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model




4. Press the Up Key to set the value to 5. The setting will be validated automatically if no change is made for five seconds. The *d.c.c.t* decimal point position setting will be displayed again.

Note Press the Mode Key to enter the setting immediately. The next parameter will be displayed for setting.


Set Value LED Display Model

Basic Model



When no operation is executed for five seconds

Set Value LED Display Model Basic Model



LnSH

Upper-limit Compensation Value


LnSL

Lower-limit Compensation Value



FUNCTION

The upper- and lower-limit values of the sensor can be shifted. If both the upper- and lower-limit values are shifted by 2°C each, for example, a process value of 200°C will be treated as 202°C after compensation.

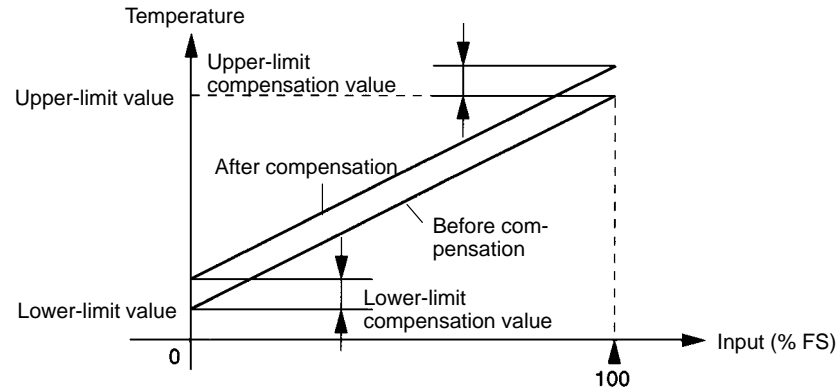

SETTING

Set value	Unit	Default
-1999 to 9,999	---	0

**SETTING
EXAMPLE**

Follow the steps described below to set both the upper- and lower-limit compensation values to 2.

Set Value LED Display Model

Basic Model



1, 2, 3...

1. Press the Mode Key for more than one second while the *oPt* option menu is displayed. The *RuG* average processing setting will appear.

Set Value LED Display Model



Basic Model



2. Press the Mode Key twice to display the *LnSH* upper-limit compensation value setting.

Set Value LED Display Model

Basic Model



- Press the Shift Key to display present set value 0000 for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model




- Press the Up Key to set the value to 2. The setting will be validated automatically if no change is made for five seconds. The LnSH upper-limit compensation value setting will be displayed again.

Note Press the Mode Key to enter the setting immediately. The next parameter will be displayed for setting.

Set Value LED Display Model



Basic Model



- Press the Mode Key to display the LnSL lower-limit compensation value setting.

Set Value LED Display Model

Basic Model



- Press the Shift Key to display present set value 0000 for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model



- Press the Up Key to set the value to 2. The setting will be validated automatically if no change is made for five seconds. The LnSH upper-limit compensation value setting will be displayed again.

Note Press the Mode Key to enter the setting immediately. The next parameter will be displayed for setting.

Set Value LED Display Model



Basic Model



When no operation is executed for five seconds

Set Value LED Display Model

Basic Model



H45

Hysteresis

FUNCTION



SETTING




REFERENCE

- The hysteresis can be set in the option menu to prevent “chattering” of the output if the measured value fluctuates in the vicinity of the setting values.
- The hysteresis can be set within a range of 1 and 9999 digits for four consecutive digits beginning with the leftmost digit regardless of the decimal point.
- The value set to 0 is regarded as 1.
- The decimal point position set in the scaling menu becomes valid.

Setting range	Unit	Default
1 to 9999	---	1

If the comparative output is a level output, however, the hysteresis will be enabled when the measured value starts to become smaller than the HH, H, LL, and L setting values.


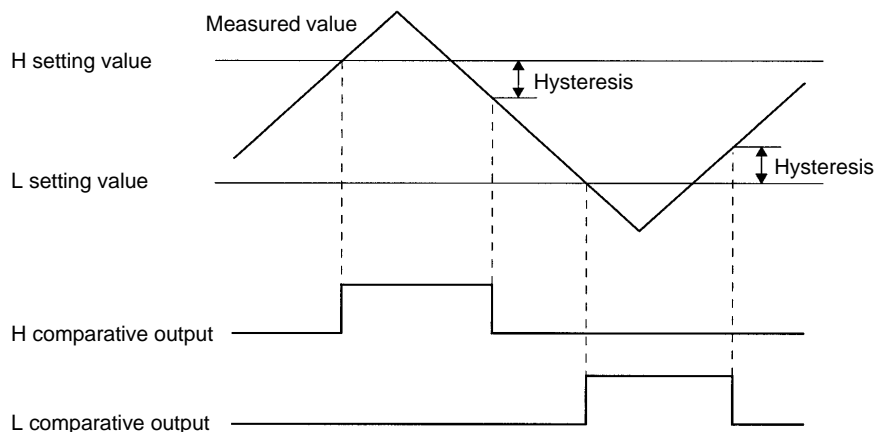


MODELS

This setting is only available for the K3NH with the Comparative Output Unit.


SETTING EXAMPLE

Follow the steps described below to set the hysteresis to 30.

Set Value LED Display Model**Basic Model**

1, 2, 3...



1. Press the Mode Key for more than one second while the $\bar{d}Pt$ option menu is displayed. The R_{UG} average processing setting will appear.

Set Value LED Display Model**Basic Model**

2. Repeatedly press the Mode Key until the *HYS* hysteresis setting is displayed.

Set Value LED Display Model

Basic Model



3. Press the Shift Key to display the prior set value *000* for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model



4. Press the Up and Shift Keys to set the value to *0030*. The setting will be validated automatically if no change is made for five seconds. The *HYS* hysteresis setting will be displayed again.

Note Press the Mode Key to enter the set value immediately. The next parameter will be displayed for setting.

Set Value LED Display Model


Basic Model



When no operation is executed for five seconds

Set Value LED Display Model

Basic Model




C-OUT

Comparative Output Pattern

FUNCTION



SETTING



REFERENCE

- The pattern of HH, H, L, LL, and PASS comparative outputs is set in the option menu.

Setting	Default
nōnRL: Standard output	nōnRL
ẼōnE: Zone output	
LEuEL: Level output	

Standard Output

H or HH Comparative Output:


Turns ON when the measured value is larger than the H or HH setting value.

PASS Output:

Turns ON when LL, L, H, and HH comparative outputs are all OFF.

L or LL Comparative Output:

Turns ON when the measured value is smaller than the L or LL setting value.

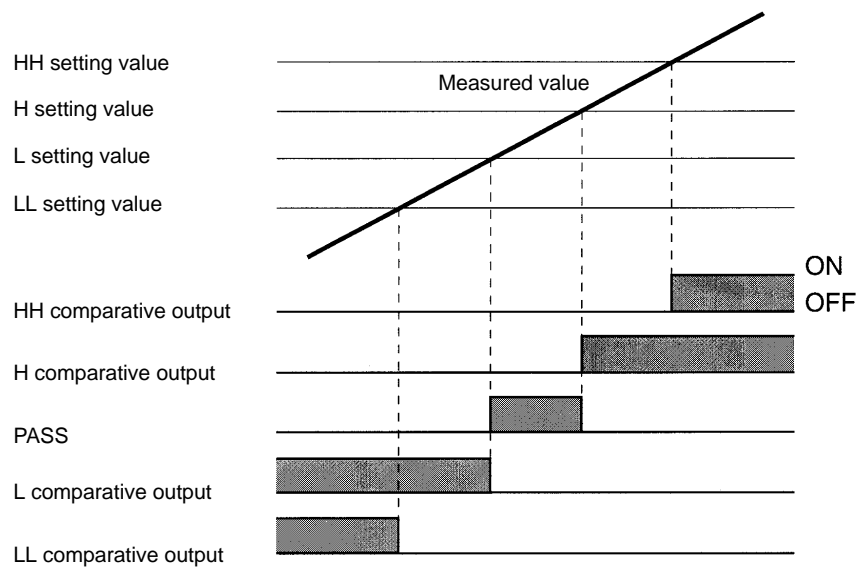


Level Output

LL, L, H, or HH Comparative Output:

Turns ON when the measured value exceeds the LL, L, H, or HH setting value.

PASS Output:

Turns ON when the LL, L, H, and HH comparative outputs are all OFF.

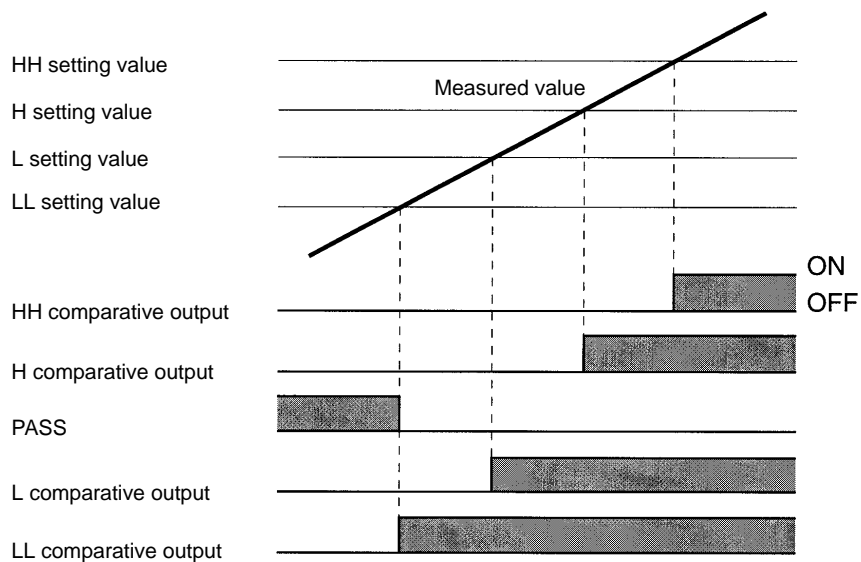**Zone Output**

HH Comparative Output:

Turns ON when the measured value exceeds the HH setting value.

H Comparative Output:

Turns ON when the measured value is between the H and HH setting values.

PASS Output:

Turns ON when the measured value is between the L and H setting values.

L Comparative Output:


Turns ON when the measured value is between the LL and L setting values.

LL Comparative Output:

Turns ON when the measured value falls below the LL setting value.

Be sure to set the setting values so they satisfy the following formula:

$$LL < L < H < HH$$

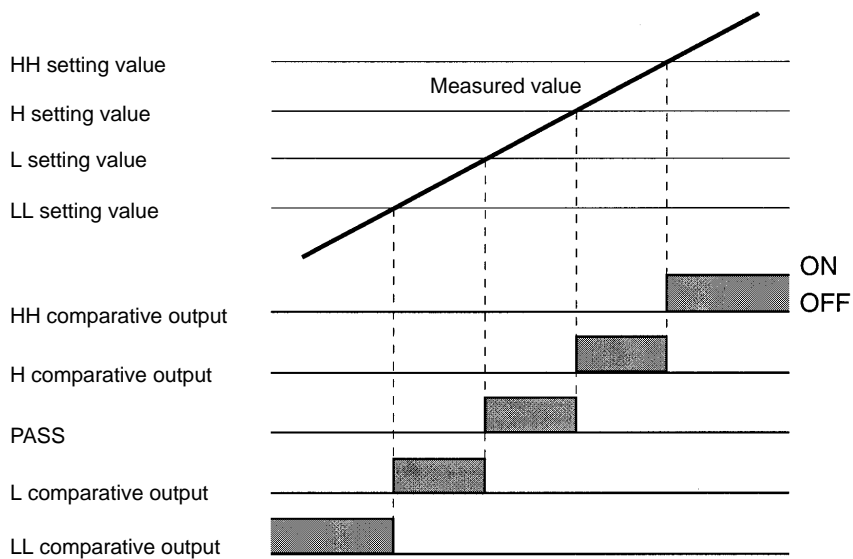



MODELS

This setting is only available for the K3NH with the Comparative Output Units.

SETTING EXAMPLE

Follow the steps described below to set the comparative output pattern to level output.

Set Value LED Display Model

Basic Model



- 1, 2, 3... 1. Press the Mode Key for more than one second while the $\bar{d}Pt$ option menu is displayed. The R_{UG} average processing setting will appear.

Set Value LED Display Model



Basic Model



2. Repeatedly press the Mode Key until the $\bar{C}-\bar{d}Ut$ comparative output pattern setting is displayed.

Set Value LED Display Model



Basic Model



3. Press the Shift Key to display the prior setting $n\bar{d}RL$ for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model




4. Press the Up Key twice to display $LEuEL$. The setting will be validated automatically if no change is made for five seconds. The $\bar{C}-\bar{d}Ut$ comparative output pattern setting will be displayed again.

Note Press the Mode Key to enter the setting immediately. The next parameter will be displayed for setting.

Set Value LED Display Model


Basic Model



When no operation is executed for five seconds

Set Value LED Display Model

Basic Model



StdbY

Standby Sequence

When the K3NH is tuned on, the K3NH will have no output until the measured value is within the PASS range. This function avoids unnecessary output until the output is within the measurement range after the power is turned ON.

Setting	Unit	Default
ON/OFF	---	OFF


This setting is only available for the K3NH with the Comparative Output Units.

SETTING
EXAMPLE

Follow the steps described below to set the standby sequence to ON.

Set Value LED Display Model

Basic Model



- 1, 2, 3... 1. Press the Mode Key for more than one second while the $\bar{d}Pt$ option menu is displayed. The RnU average processing setting will appear.

Set Value LED Display Model



Basic Model



2. Repeatedly press the Mode Key until the $StdbY$ standby sequence setting is displayed.

Set Value LED Display Model



Basic Model



3. Press the Shift Key to display present set value $\bar{d}FF$ for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model





4. Press the Up Key to set the value to $\bar{d}n$. The setting will be validated automatically if no change is made for five seconds. The $StdbY$ standby sequence setting will be displayed again.

Note Press the Mode Key to enter the setting immediately. The next parameter will be displayed for setting.


Set Value LED Display Model

Basic Model



When no operation is executed for five seconds

Set Value LED Display Model Basic Model



L5Et.H

Upper Limit (H) of Linear Output Range

L5Et.L


Lower Limit (L) of Linear Output Range



FUNCTION

Linear output setting is made in the option menu to enable the K3NH to have voltage or current output in proportion to the change in display value.

- The maximum and minimum values of linear output are set in this parameter.

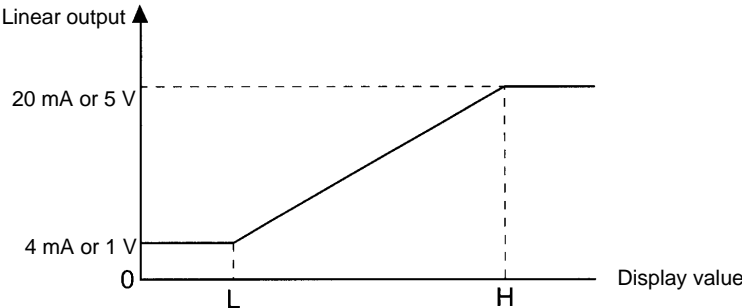

- L can be greater or less than H.
- L cannot be the same as H, otherwise H will be automatically set to a value obtained by adding 1 to L.
- The teaching function can be used for setting linear output ranges.



SETTING



REFERENCE



MODELS

Setting range	Default	
-1999 to 9999	H linear output range	9999
	L linear output range	-1999

Refer to 5-1 Teaching Function.

This setting is available for the K3NH with the Linear Output Board.

SETTING
EXAMPLE

Follow the steps described below to set the following.

H: 100

L: 0

Set Value LED Display Model



Basic Model



- 1, 2, 3... 1. Press the Mode Key for more than one second while the $\bar{d}Pt$ option menu is displayed. The RuG average processing setting will appear.

Set Value LED Display Model



Basic Model



2. Repeatedly press the Mode Key until the $LSEt.H$ H linear output range setting is displayed.

Set Value LED Display Model

Basic Model



3. Press the Shift Key to display the prior set value 9999 for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model



4. Press the Up and Shift Keys to set the value to 100 . The setting will be validated automatically if no change is made for five seconds. The $LSEt.H$ H linear output range setting will be displayed again.

Note Press the Mode Key to enter the set value immediately. The next parameter will be displayed for setting.

Set Value LED Display Model


Basic Model



5. Press the Mode Key to display the $LSEt.L$ L linear output range setting.

Set Value LED Display Model

Basic Model



6. Press the Shift Key to display the prior set value -1999 for changing. The PROG indicator will flash.

Set Value LED Display Model


Basic Model



7. Press the Up and Shift Keys to set the value to 0000. The setting will be validated automatically if no change is made for five seconds. The LSEt.L L linear output range setting will be displayed again.


Note Press the Mode Key to enter the set value immediately. The next parameter will be displayed for setting.

Set Value LED Display Model Basic Model




When no operation is executed for five seconds

Set Value LED Display Model Basic Model



r-L

Remote/Local Programming



FUNCTION



SETTING



MODELS

- The K3NH can be set to remote or local mode in the option menu. The K3NH in remote mode is operated through the host computer and the K3NH in local mode is operated through the front panel key input.

Setting	Default
Remote: r \bar{n} L	L \bar{L} L
Local: L \bar{L} L	


This setting is available for the K3NH with the Communications Output Board.

SETTING
EXAMPLE

Follow the steps described below to set the K3NH to remote programming.

Set Value LED Display Model

Basic Model




1, 2, 3...

- Press the Mode Key for more than one second while the $\bar{d}Pt$ setup menu is displayed. The RuG setting will appear.

Set Value LED Display Model


Basic Model



- Repeatedly press the Mode Key until the r-L remote/local setting is displayed.

Set Value LED Display Model



Basic Model



- Press the Shift Key to display the prior setting L \bar{L} L for changing. The PROG indicator will flash.

Set Value LED Display Model



Basic Model



- Press the Up Key to display r \bar{n} L.

Set Value LED Display Model


Basic Model



5. The setting will be validated automatically if no change is made for five seconds. The R_{UL} average processing setting will be displayed again.

Note Press the Mode Key to enter the setting immediately. The $r-l$ remote/local setting will be displayed again.


Set Value LED Display Model Basic Model



3-3 Protect Mode


3-3-1 Selecting Protect Mode


- The K3NH in RUN mode will go into protect mode if the Escape and Up Keys are pressed for more than 1 second.
- The K3NH in protect mode will go into RUN mode if the Escape Key is pressed.

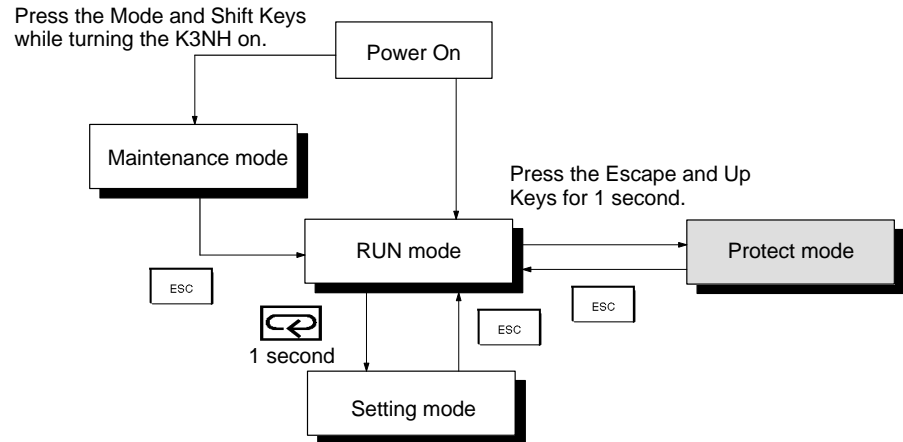

- If the Mode Key is pressed for more than one second while a menu is displayed, a parameter will be displayed.
- The parameter changes whenever the Mode Key is pressed.
- If the Shift Key is pressed while a parameter is displayed, the parameter will be ready to change.
- Press the Up Key to change parameters.

3-3-2 Menu Overview

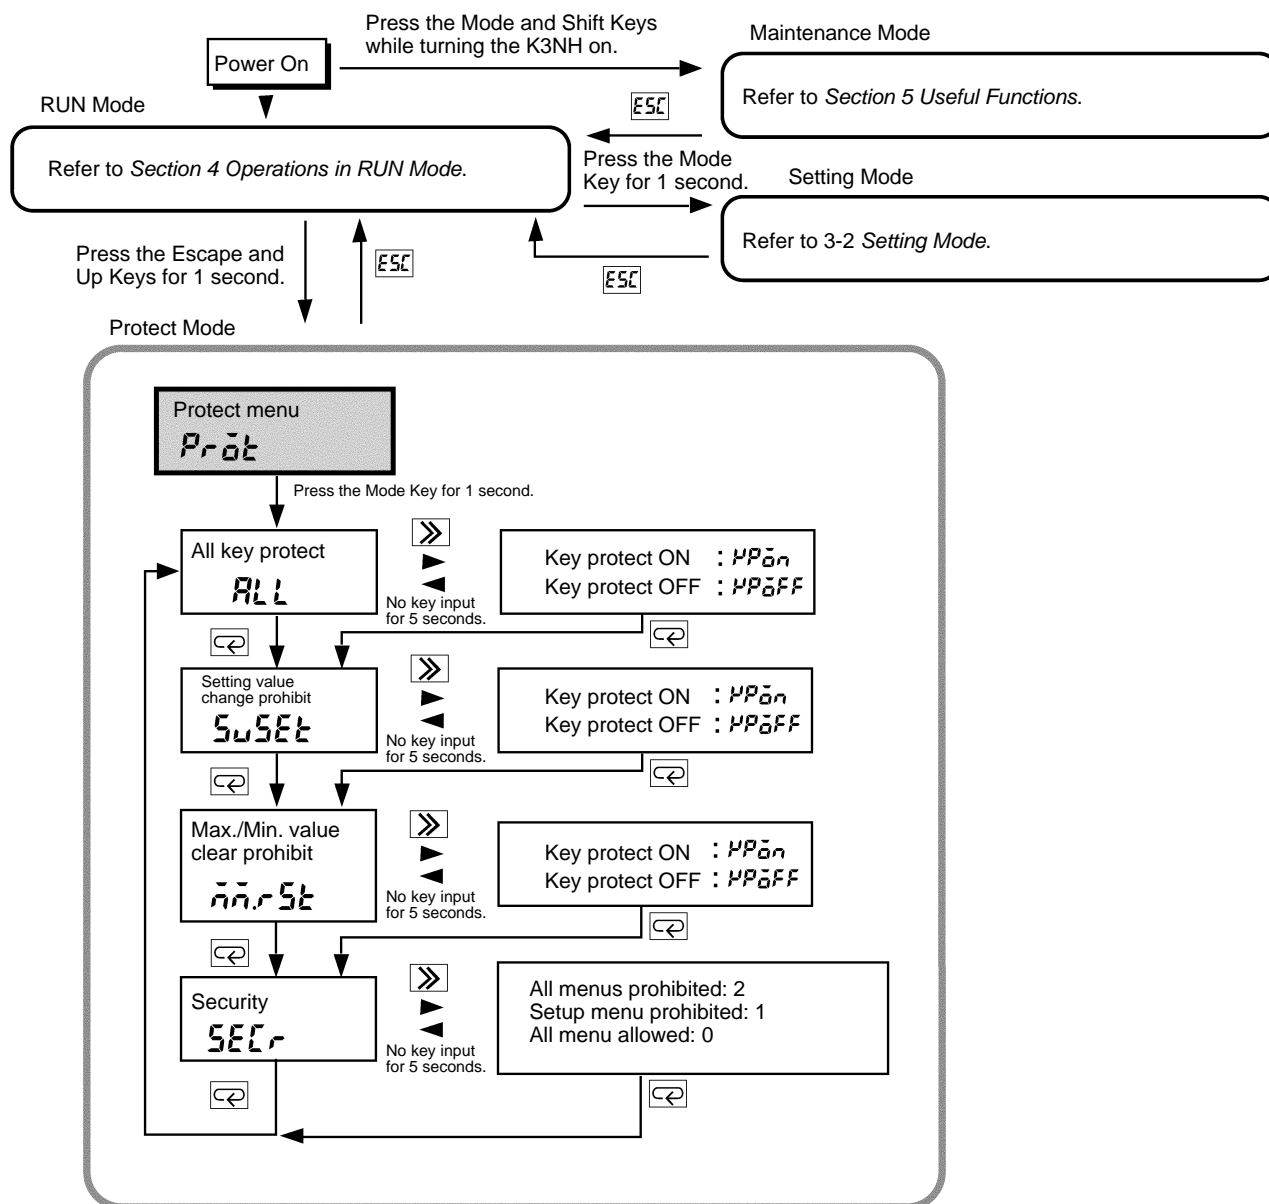

3-3-3 Protect Menu ($P_{r\bar{o}t}$)**ALL**All Key Protect

FUNCTION



SETTING

- The operation of all keys can be prohibited in the protect menu.


Setting	Default
$HP_{\bar{o}n}$: Key protect ON $HP_{\bar{o}FF}$: Key protect OFF	$HP_{\bar{o}FF}$

**SETTING
EXAMPLE**

Follow the steps described below to set the key protect to ON.

Set Value LED Display Model



Basic Model



- 1, 2, 3... 1. Press the Mode Key for more than one second while the $P_{r\bar{o}t}$ protect menu is displayed. The ALL all key protect setting will appear.

Set Value LED Display Model



Basic Model



2. Press the Shift Key to display the prior setting $HP_{\bar{o}FF}$ for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model





3. Press the Up Key to display $HP_{\bar{o}n}$. The setting will be validated automatically if no change is made for five seconds. The ALL all key protect setting will be displayed again.


Note Press the Mode Key to enter the setting immediately. The next parameter will be displayed for setting.

Set Value LED Display Model


Basic Model



When no operation is executed for five seconds




5u5Et

Setting Value Change Prohibit

FUNCTION



SETTING



REFERENCE



MODELS

- The setting value change of the K3NH in RUN mode with the front-panel key inputs can be prohibited in the protect menu.

Setting	Default
<i>PPon</i> : Key protect ON <i>PPOFF</i> : Key protect OFF	<i>PPOFF</i>

Refer to 4-1 Checking and Changing Setting Values.



This setting is only available for the K3NH with the Comparative Output Unit.

**SETTING
EXAMPLE**

Follow the steps described below to set the setting value change prohibit to ON.

Set Value LED Display Model


Basic Model



- 1, 2, 3...
- Press the Mode Key for more than one second while the *PrOt* protect menu is displayed. The *ALL* all key protect setting will appear.

Set Value LED Display Model



Basic Model



- Press the Mode Key to display the *5u5Et* setting value prohibit setting.

Set Value LED Display Model



Basic Model



- Press the Shift Key to display the prior setting *PPOFF* for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model





4. Press the Up Key to display HP_{on} . The setting will be validated automatically if no change is made for five seconds. The $SuSEt$ setting value prohibit setting will be displayed again.

Note Press the Mode Key to enter the setting immediately. The next parameter will be displayed for setting.

Set Value LED Display Model

Basic Model

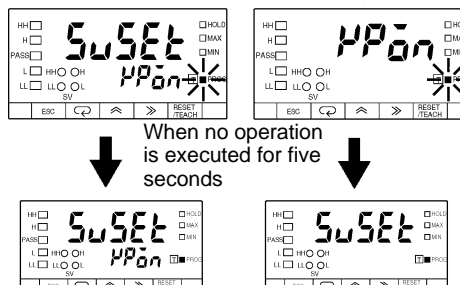




Maximum/Minimum Value Clear Prohibit



FUNCTION



SETTING



REFERENCE

- The resetting of maximum and minimum values with key input can be prohibited in the protect menu. However, the resetting of maximum and minimum values with external signal input is permitted.

Setting	Default
$PP_{\bar{O}n}$: Key protect ON $PP_{\bar{O}FF}$: Key protect OFF	$PP_{\bar{O}FF}$



Refer to 4-2 Checking and Resetting of Maximum and Minimum Values.

SETTING EXAMPLE

Follow the steps described below to set the maximum/minimum value clear prohibit to ON.

Set Value LED Display Model


Basic Model



- 1, 2, 3...
- Press the Mode Key for more than one second while the $Pr_{\bar{O}t}$ protect menu is displayed. The ALL all key protect setting will appear.

Set Value LED Display Model



Basic Model



- Repeatedly press the Mode Key until the $\bar{n}\bar{n}.r5t$ maximum/minimum value clear prohibit setting is displayed.

Set Value LED Display Model

Basic Model



- Press the Shift Key to display the prior setting $PP_{\bar{O}FF}$ for changing. The PROG indicator will flash.

Set Value LED Display Model

Basic Model





4. Press the Up Key to display $\mu P \bar{O} n$. The setting will be validated automatically if no change is made for five seconds. The $\bar{n} \bar{n} . r S t$ maximum/minimum value clear prohibit setting will be displayed again.


Note Press the Mode Key to enter the setting immediately. The next parameter will be displayed for setting.

Set Value LED Display Model

Basic Model



When no operation is executed for five seconds



SECr

Security

FUNCTION



SETTING


- Settings in setting mode can be prohibited in the protect menu.
- The following table shows what set values for menus can be prohibited. The default is 0.

Menu	Set value		
	0	1	2
Setting value			Prohibited
Scaling			Prohibited
Setup		Prohibited	Prohibited
Option			Prohibited



- The value changes in the following order with the Up Key: 0, 1, 2, and 0

**SETTING
EXAMPLE**



Follow the steps described below to set the security setting to 1.

Set Value LED Display Model**Basic Model****1, 2, 3...**



1. Press the Mode Key for more than one second while the *Pröt* protect menu is displayed. The *ALL* all key protect setting will appear.

Set Value LED Display Model**Basic Model**

2. Repeatedly press the Mode Key until the *SECr* security setting is displayed.

Set Value LED Display Model**Basic Model**

3. Press the Shift Key to display the prior set value *0* for changing. The PROG indicator will flash.


Set Value LED Display Model**Basic Model**

4. Press the Up Key to display *1*. The setting will be validated automatically if no change is made for five seconds. The *SEC* security setting will be displayed again.

Note Press the Mode Key to enter the setting immediately. The next parameter will be displayed for setting.

Set Value LED Display Model

Basic Model

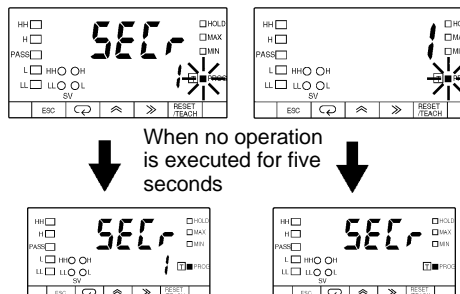

When no operation
is executed for five
seconds

SECTION 4

Operations in RUN Mode

This section provides instructions for operating the K3NH in RUN mode.


4-1	Displaying and Changing Setting Values	68
4-1-1	Displaying Setting Values	68
4-1-2	Changing Setting Values	68
4-2	Displaying and Resetting of Maximum and Minimum Values	71
4-2-1	Displaying Maximum and Minimum Values	71
4-2-2	Resetting Maximum and Minimum Values	71
4-3	External Input Signals	72
4-3-1	RESET	72
4-3-2	HOLD	72

4-1 Displaying and Changing Setting Values

4-1-1 Displaying Setting Values

Basic Model

- When the Mode Key is pressed in RUN mode, the K3NH displays a setting value on the PV display (in the order of HH, H, L, and LL).
- While the setting value is displayed, the corresponding SV display status indicator is lit.
- Unless another operation key is pressed within five seconds after the setting value is displayed, the process, maximum, or minimum value is displayed again.

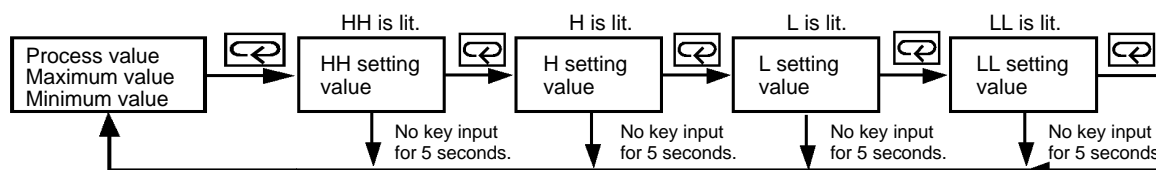

Set Value LED Display Model

- The setting value appears on the SV display and the corresponding SV display status indicator is lit while the process, maximum, or minimum value is displayed on the PV display
- When the Mode Key is pressed, the K3NH displays a setting value (in the order of HH, H, L, and LL) on the SV display.


4-1-2 Changing Setting Values

- Setting values can be prohibited against change when key protect or setting value change prohibit is ON in protect mode.
- Select the setting value to be changed with the Mode Key.
- All digits will be displayed and ready for changing if the Shift Key is pressed.
- Press the Up and Shift Keys to change the displayed setting value. The input will be entered if nothing else is input within five seconds. The input is entered immediately by pressing the Mode Key.
- The next setting value will be displayed and ready for changing if the Mode Key is pressed. If nothing else is input within five seconds, the setting value will be entered and the previous setting value will be displayed.
- The setting value can be changed through communications if the K3NH is a model with a communications function.


**SETTING
EXAMPLE**

Basic Model


Follow the steps below to change the H setting value from 600 to 700 while the process value is displayed in RUN mode.



- 1, 2, 3...**
1. Press the Mode Key to display the HH setting value and to light the HH indicator of the SV display status indicators.



2. Press the Mode Key again to display the H setting value H and light the H indicator.



3. Press the Shift Key to display all the digits of the prior setting value 0600 for changing.




4. Press the Up and Shift Keys to set the value to 0700.



5. The input will be entered if nothing else is input within five seconds.
or Press the Mode Key to display the L setting value for changing. The H setting value will appear again if nothing else is input within five seconds.



6. To return to the process value display, perform one of the following.
 - Repeatedly press the Mode Key until the process value appears.
 - Leave the K3NH with no key input for five seconds.



**SETTING
EXAMPLE**

**Set Value LED Display
Model**

Follow the steps below to change the H setting value from 600 to 700 while the process value is displayed in RUN mode, provided that the HH setting value is already displayed on the SV display.



- 1, 2, 3...** 1. Press the Mode Key to display the H setting value and to light the H indicator of the SV display status indicators.




2. Press the Shift Key to display all the digits of the setting value 0600 for changing.



3. Press the Up and Shift Keys to set the value to 0700.



4. The input will be entered if nothing else is input within five seconds.
or Press the Mode Key to display the L setting value for changing. The H setting value will appear again if nothing else is input within five seconds.




4-2 Displaying and Resetting of Maximum and Minimum Values

The maximum and minimum values are refreshed automatically while the K3NH is in measurement operation.

4-2-1 Displaying Maximum and Minimum Values

- The Escape Key is used to select the process, maximum, or minimum value to be displayed on the PV display in RUN mode.
- The corresponding SV display indicator (i.e., the MAX or MIN indicator) is lit while the maximum or minimum value is displayed.

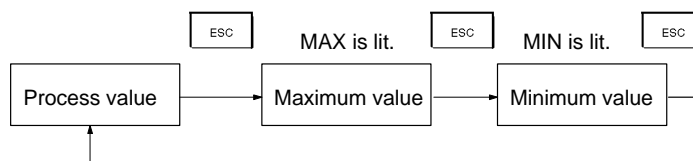

4-2-2 Resetting Maximum and Minimum Values

- The maximum and minimum values are reset when the K3NH is turned on, set to RUN mode, or reset.
- The K3NH will be reset when one of the following is performed.
 - The Reset/Teach Key is pressed for more than one second while the maximum or minimum value is displayed.
 - The external RESET input signal is turned ON.
 - The K3NH receives the reset command through communications.
- When the K3NH is reset, the maximum and minimum values are set to the process value.


Note The K3NH cannot be reset with the Reset/Teach Key if the maximum/minimum value clear prohibit is ON in protect mode.

SETTING EXAMPLE

- 1, 2, 3... 1. The process value 401 is displayed.

Set Value LED Display Model


Basic Model




2. Press the RESET/TEACH Key to display the maximum value 1024 and light the MAX indicator.

Set Value LED Display Model


Basic Model



- Press the RESET/TEACH Key to set the maximum and minimum values to the process value 401.

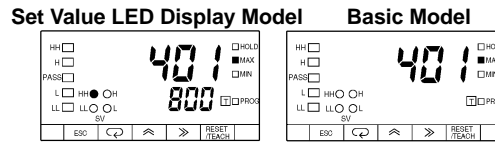


- Press the Escape Key to check that the minimum value is set to 401.

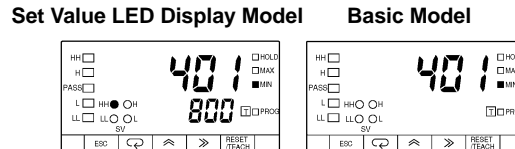

4-3 External Input Signals


4-3-1 RESET

- Refer to 4-2 *Displaying and Resetting of Maximum and Minimum Values* for the function of this signal.
- The following graph shows the operation timing of the signal.

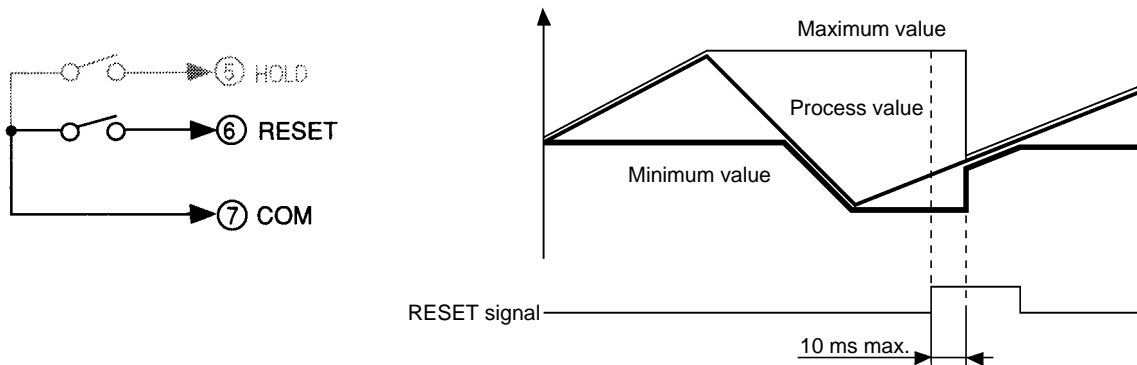

4-3-2 HOLD

- The K3NH will stop the measurement if the HOLD input is ON.
- When the HOLD input is ON, the K3NH will retain the process value, output, and BCD data effective immediately before the HOLD input.
- The HOLD indicator is lit while HOLD input is ON.

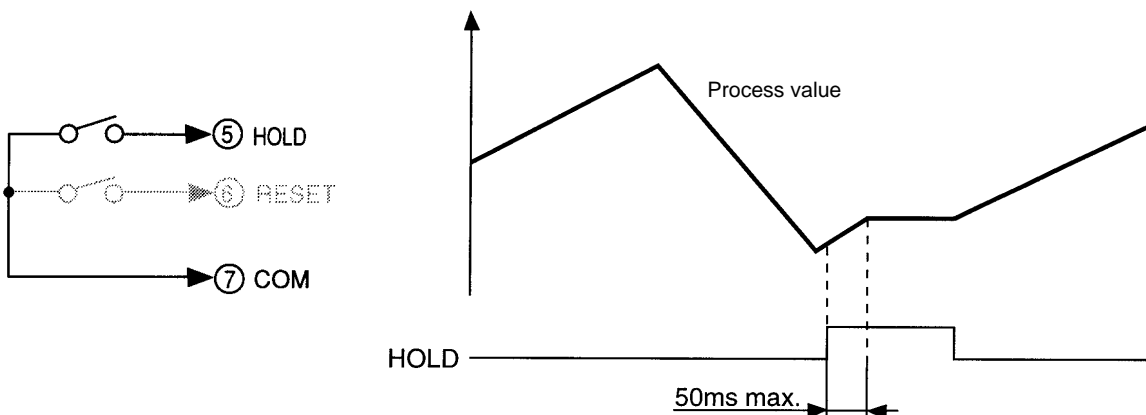

SECTION 5

Useful Functions

This section provides information on the teaching function, output test, and maintenance mode.

5-1	Teaching Function	74
5-1-1	Set Value	74
5-1-2	Linear Output Range	75
5-2	Output Test	76
5-3	Maintenance Mode	77
5-3-1	Maintenance Mode	77
5-3-2	Initialization	77
5-3-3	Field Calibration	78
5-3-4	Thermocouple Calibration	79
5-3-5	Temperature-resistance Thermometer Calibration	85
5-3-6	Current Input Calibration	88
5-3-7	Voltage Input Calibration	89

5-1 Teaching Function

- The K3NH is provided with a teaching function that can set an actual measured value as a set value without any front panel key input.

This function is useful for setting parameters while checking the operating status of the K3NH.

- The teaching function can be used to set the setting, scaling values, and linear output range. The TEACH indicator will be lit if a parameter that can use the teaching function is displayed.

5-1-1 Set Value

- A setting value can be set with the actual input instead of key input in the setting mode.
- Follow the steps below to teach the setting value.



- 1, 2, 3...**
1. Press the RESET/TEACH Key for more than one second while the parameter is displayed. The process value will be displayed and the teaching indicator will flash.
 2. Press the RESET/TEACH Key again to retrieve the process value immediately before the key was pressed as a set value. The teaching indicator will be lit and the parameter will be displayed. Press the Escape Key to interrupt teaching.

SETTING EXAMPLE

Follow the steps described below to set the HH set value by using the teaching function.

Set Value LED Display Model


Basic Model



- 1, 2, 3...**
1. Press the RESET/TEACH Key for more than one second while the parameter is displayed. The process value will be displayed and the teaching indicator will flash.

Set Value LED Display Model


Basic Model



2. Press the RESET/TEACH Key again to retrieve the process value immediately before the key was pressed as a set value for changing. The teaching indicator will be lit and the parameter is displayed.

Set Value LED Display Model

Basic Model



5-1-2 Linear Output Range

The teaching function can be also used to set the linear output range of the K3NH with the Linear Output Board.


- The H and L linear output ranges can be set using the actual measured value instead of key input in the option menu.
- Follow the steps below to teach the setting value.

- 1, 2, 3...** 1. Press the RESET/TEACH Key for more than one second while the parameter is displayed. The process value will be displayed and the teaching indicator will flash.
2. Press the RESET/TEACH Key again to retrieve the process value immediately before the key was pressed as a set value. The teaching indicator will be lit and the parameter will be displayed. Press the Escape Key to interrupt teaching.

SETTING EXAMPLE


Follow the steps described below to set the H linear output range by using the teaching function.

Set Value LED Display Model Basic Model




- 1, 2, 3...** 1. Press the RESET/TEACH Key for more than one second while the parameter is displayed. The process value will be displayed and the teaching indicator will flash.

Set Value LED Display Model Basic Model



2. Press the RESET/TEACH Key again to retrieve the process value immediately before the key was pressed as a set value for changing. The teaching indicator will be lit and the parameter will be displayed. Press the Escape Key to interrupt teaching.

Set Value LED Display Model Basic Model




5-2 Output Test

This function is convenient for checking a system to which the K3NH is connected, especially when some inputs cannot be operated. The K3NH simulates an input signal to check the output conditions.

Note The K3NH has output according to the simulated input in this mode. If there is any device connected to the output of the K3NH, be sure that the output will not have a negative influence on the device before testing the system.

- Follow the steps described below to perform the test.

- 1, 2, 3...**
1. While the K3NH is in RUN mode, press the Mode Key for more than one second to set the K3NH to the setting mode.
 2. Repeatedly press the Mode Key until *LES* output test setting is displayed.

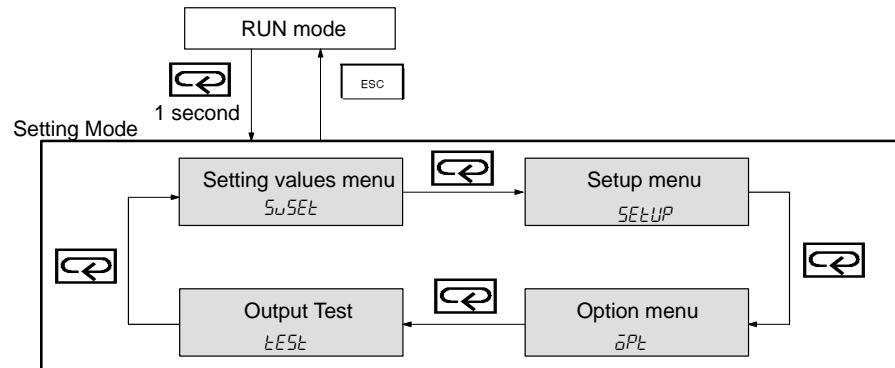

3. Press the Mode Key for more than one second to display 0, which is a simulated input value.
 4. The simulated input value increases when the Up Key is pressed. Comparative outputs are output according to the output pattern that has been preset.
 5. The simulated input value decreases when the Shift Key is pressed. Comparative outputs are output according to the output pattern that has been preset.
 6. Press the Escape Key after testing. The *LES* output test setting will be displayed again.
 7. Press the Escape Key to return to the RUN mode.
- To change the simulated input value continuously, keep pressing the Up or Shift Key.


5-3 Maintenance Mode

The set values of the K3NH can be initialized and field calibration of the K3NH is possible in maintenance mode. The operations of the K3NH in this mode are described below.

5-3-1 Maintenance Mode

- The K3NH will be in maintenance mode if the Mode and Shift Keys are simultaneously pressed while the K3NH is turned on.
- The K3NH in maintenance mode will go into RUN mode if the Escape Key is pressed.

Press the Mode and Shift Keys while turning the K3NH on.

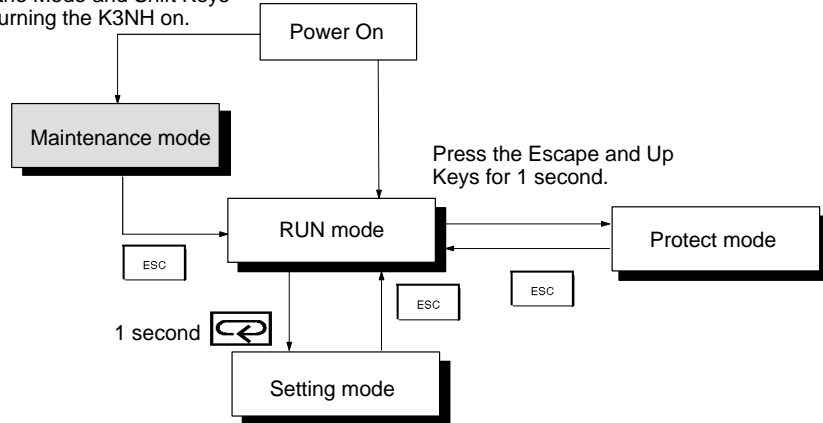



5-3-2 Initialization

Follow the steps described below to reset the set values of the K3NH to factory-set values.

- 1, 2, 3...**
1. Press the Mode and Shift Keys simultaneously while turning the K3NH on. The $\bar{n}A_{nt}$ maintenance mode setting will be displayed.

Set Value LED Display Model



Basic Model



2. Press the Mode Key for more than one second. The $rE-\bar{L}n$ initialization setting will be displayed.

Set Value LED Display Model



Basic Model



3. Press the Up Key to display $n\bar{o}$.


Set Value LED Display Model

Basic Model



4. Press the Up Key to display *YES*. Press the Mode Key to initialize all set values. The K3NH will go into RUN mode.

Set Value LED Display Model Basic Model

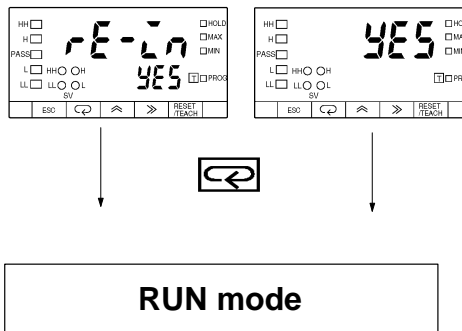


5-3-3 Field Calibration

Calibration is to be performed when adjustment is required for display accuracy exceeding the specified value. Follow the procedure below when calibration is required.

Be sure to conduct an accuracy test after calibration.

The following is the configuration of parameters for the user's reference.

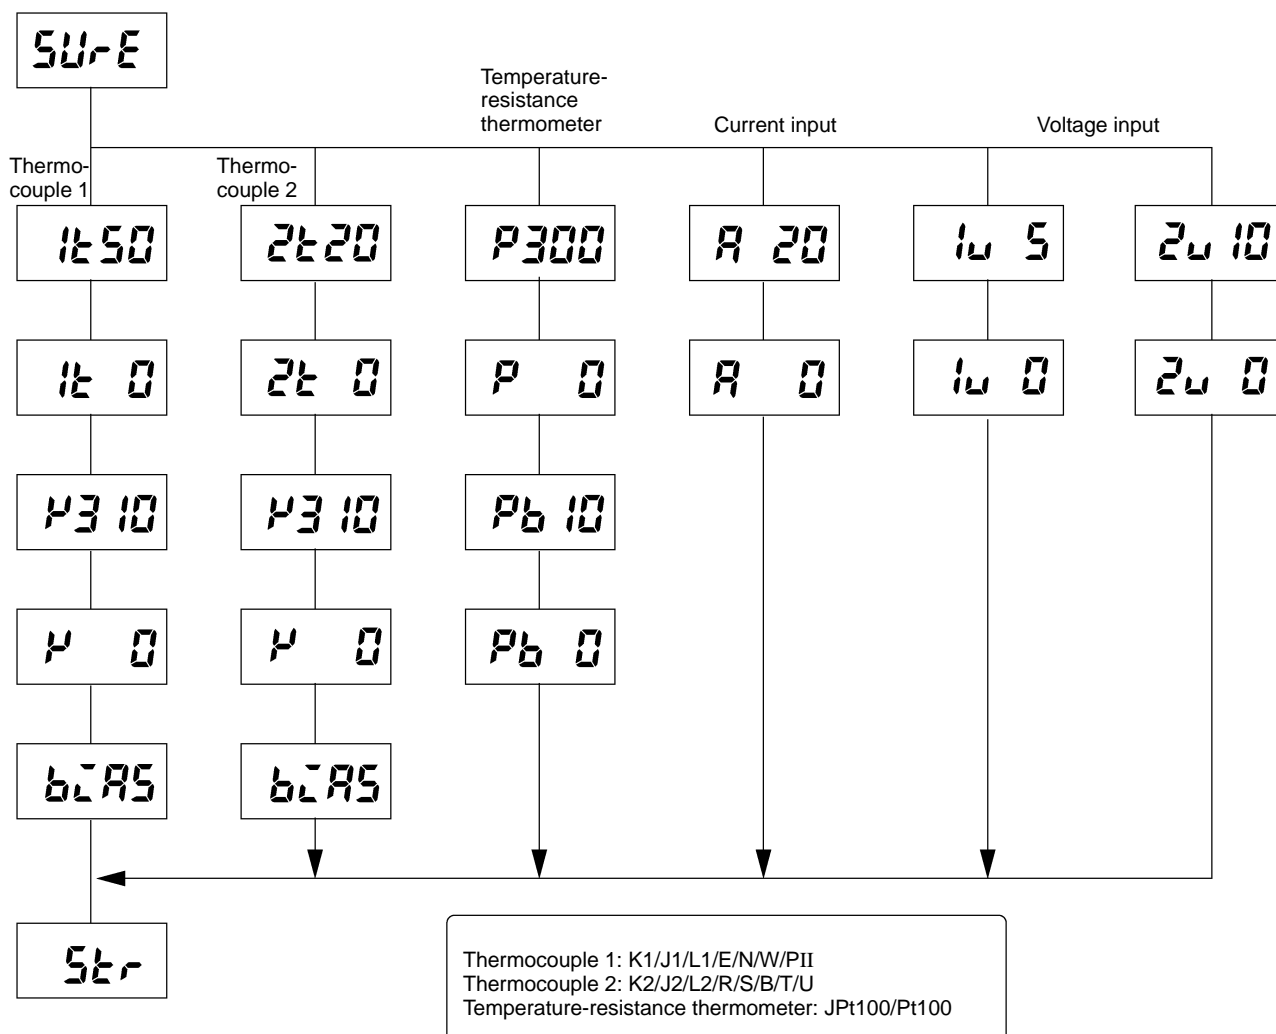



- Only input set with the input type parameter in setup mode can be the object of input calibration. Press the Mode Key for approximately one second to tentatively register the parameter data of all calibration items.
- The data registration setting *Str* does not appear unless all calibration items are tentatively registered.

Procedure for Field Calibration

- 1, 2, 3... 1. Press the Mode and Shift Keys simultaneously while turning the K3NH on to display *mant* maintenance mode setting.

Set Value LED Display Model



Basic Model



2. Press the Mode Key for more than one second to display *re-tn* set value initialization setting.

Set Value LED Display Model

Basic Model



3. Press the Mode Key to display the *calib* field calibration setting.

Set Value LED Display Model



Basic Model



4. Press the Shift Key to display *no*.

Set Value LED Display Model



Basic Model



5. Press the Up Key to display *YES*. Press the Mode Key to select the calibration item.

Set Value LED Display Model

Basic Model



User calibration


5-3-4 Thermocouple Calibration

- There are two calibration methods. One applies to thermocouple group 1 (i.e., K1, J1, L1, E, N, W, and PLII) and the other applies to thermocouple group 2 (K2, J2, L2, R, S, B, T, and U).

- Do not touch input terminals 3 or 4 or compensating conductor during calibration.


Preparation

- Connect an STV (standard voltage/current generator) to input terminals 3 and 4.
- Prepare a cold junction compensator with a built-in thermocouple that is the same type as the calibrating thermocouple, and set the compensator to 0°C with the built-in thermocouple disabled (i.e., the terminals left open).

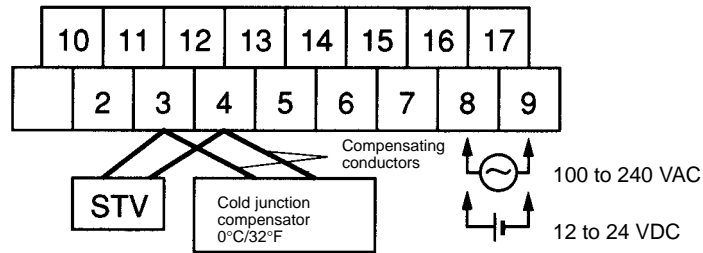

Note Connection of Cold Junction Compensator

The thermocouple cannot be calibrated correctly if the connecting points of the compensating conductors come into contact with the human body. Therefore, be sure to enable the built-in thermocouple by short-circuiting the thermocouple or disable the thermocouple by keeping the thermocouple terminals open to connect or disconnect the cold junction compensator as shown in the following illustration.


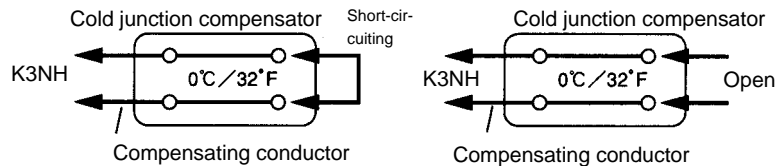


Thermocouple Group 1 Calibration

- 1, 2, 3... 1. First, the *SURE* alarm display will appear. This will not appear once field calibration is performed.

Set Value LED Display Model



Basic Model



2. Press the Mode Key to display *1250*. The teaching indicator will be lit. Then calibrate the main input.

Set Value LED Display Model


Basic Model



3. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of the STV to 50 mV. The teaching indicator will flash. After the


value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model Basic Model




4. The display will change to 12.0 for 0-mV calibration. The teaching indicator will be lit.

Set Value LED Display Model Basic Model




5. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of the STV to 0 mV. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model Basic Model




6. Calibrate the cold junction compensating block next. The display will change to 43.10 for 310-mV calibration. The teaching indicator will be lit.

Set Value LED Display Model Basic Model




7. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of the STV to 310 mV. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model Basic Model



8. The display will change to 4.0 for 0-mV calibration. The teaching indicator will be lit.

Set Value LED Display Model Basic Model





9. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of the STV to 0 mV. The teaching indicator will flash. After the

value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



10. Calibrate the bias compensation value as the last item. The display will change to *bIAS*. The teaching indicator will be lit. Disconnect the STV, set the cold junction compensator to 0°C, and enable the built-in thermocouple. Be sure to disconnect the wires connected to the STV.

Set Value LED Display Model


Basic Model



11. Press the RESET/TEACH Key to display the calibration value setting. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



12. The display will change to *St-* for confirmation of the settings.

Set Value LED Display Model



Basic Model



13. Press the Shift Key to select whether or not to accept the settings.

Set Value LED Display Model



Basic Model



14. Press the Up Key to select *YES*.
15. Press the Mode Key to overwrite all calibration data and to put the K3NH into RUN mode. The calibration data will not be overwritten if *no* is selected.

Set Value LED Display Model

Basic Model





RUN mode

Thermocouple Group 2 Calibration

- 1, 2, 3... 1. First, the *SU-E* alarm display will appear. This will not appear once field calibration is performed.

Set Value LED Display Model



Basic Model



2. Press the Mode Key to display *2t 50*. The teaching indicator will be lit. Then calibrate the main input.

Set Value LED Display Model



Basic Model



3. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of the STV to 20 mV. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



4. The display will change to *2t 0* for 0-mV calibration. The teaching indicator will be lit.

Set Value LED Display Model



Basic Model



5. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of the STV to 0 mV. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than a several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



6. Calibrate the cold junction compensating block next. The display will change to *43 10* for 310-mV calibration. The teaching indicator will be lit.

Set Value LED Display Model

Basic Model




7. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of the STV to 310 mV. The teaching indicator will flash. After

the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



8. The display will change to μ 0 for 0-mV calibration. The teaching indicator will be lit.

Set Value LED Display Model



Basic Model



9. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of the STV to 0 mV. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



10. Calibrate the bias compensation value as the last item. The display will change to b_{LR}5. The teaching indicator will be lit. Disconnect the STV, set the cold junction compensator to 0°C, and enable the built-in thermocouple. Be sure to disconnect the wires connected to the STV.

Set Value LED Display Model



Basic Model



11. Press the RESET/TEACH Key to display the calibration value setting. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



12. The display will change to 5_{tr} for confirmation of the settings.

Set Value LED Display Model



Basic Model



13. Press the Shift Key to select whether or not to accept the settings.

Set Value LED Display Model


Basic Model



14. Press the Up Key to select *YES*.
15. Press the Mode Key to overwrite all calibration data and to put the K3NH into RUN mode. The calibration data will not be overwritten if *no* is selected.

Set Value LED Display Model

Basic Model




RUN mode

5-3-5 Temperature-resistance Thermometer Calibration

Preparation

- Make sure that the thickness of each connected wire is the same.
- Dial 6 in the following diagram represents a high-precision resistance box.
- Short-circuit terminals 3 and 4 with each other.


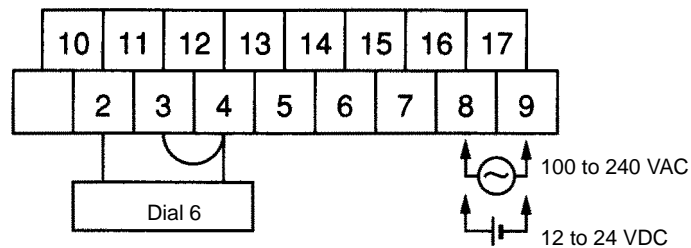


Calibration

- 1, 2, 3... 1. First, the *SU-E* alarm display will appear. This will not appear once field calibration is performed.

Set Value LED Display Model



Basic Model



2. Press the Mode Key to display *P300*. The teaching indicator will be lit. Then calibrate the main input.

Set Value LED Display Model


Basic Model



3. Press the RESET/TEACH Key to display the calibration value setting. Then set Dial 6 to 300 Ω . The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



4. The display will change to $P \square$ for 0- Ω calibration. The teaching indicator will be lit.

Set Value LED Display Model

Basic Model





Short-circuit terminals 2 to 4.


5. Press the RESET/TEACH Key to display the calibration value setting. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model

Basic Model




6. Calibrate the B-to-B' input next. The display will change to $Pb \square$ for 10- Ω calibration. Change the wiring as shown below.

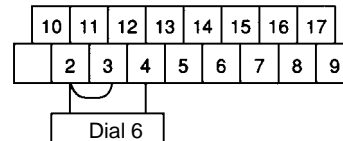

Make the wiring distance between the Dial 6 and terminals 2 and 4 as short as possible. Short-circuit terminals 2 and 3 to each other.

Set Value LED Display Model

Basic Model





Change wiring.

7. Press the RESET/TEACH Key to display the calibration value setting. Then set the Dial 6 to 10 Ω . The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.


Set Value LED Display Model

Basic Model



8. The display will change to $Pb \ 0$ for 0- Ω calibration. Short-circuit terminals 2, 3, and 4 to one another. The teaching indicator will be lit.


Set Value LED Display Model Basic Model



Short-circuit terminals 2 to 4.


9. Press the RESET/TEACH Key to display the calibration value setting. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model Basic Model




10. The display will change to St_r for confirmation of the settings.

Set Value LED Display Model Basic Model




11. Press the Shift Key to select whether or not to accept the settings.

Set Value LED Display Model Basic Model



12. Press the Up Key to select YES .
13. Press the Mode Key to overwrite all calibration data and to put the K3NH into RUN mode. The calibration data will not be overwritten if no is selected.

Set Value LED Display Model Basic Model




RUN mode

5-3-6 Current Input Calibration

Preparation

Connect an STV to input terminals 13 and 14.


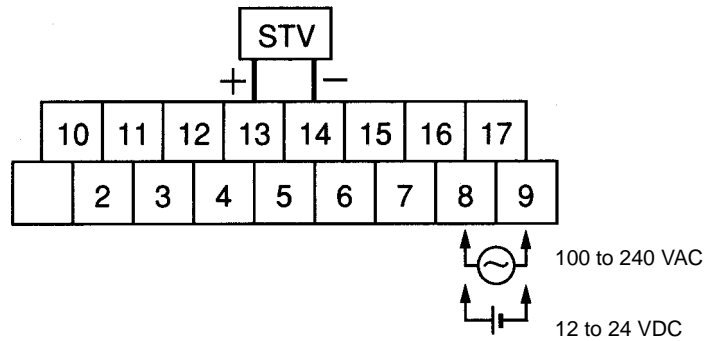


Calibration

- 1, 2, 3... 1. First, the *SURE* alarm display will appear. This will not appear once field calibration is performed.

Set Value LED Display Model



Basic Model



2. Press the Mode Key to display *A 20*. The teaching indicator will be lit.

Set Value LED Display Model



Basic Model



3. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of STV to 20 mA. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



4. The display will change to *A 0* for 0-mA calibration. The teaching indicator will be lit.

Set Value LED Display Model

Basic Model





5. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of STV to 0 mA. The teaching indicator will flash. After the val-

ue stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



6. The display will change to *St_r* for confirmation of the settings.

Set Value LED Display Model



Basic Model



7. Press the Shift Key to select whether or not to accept the settings.

Set Value LED Display Model

Basic Model





8. Press the Up Key to select *YES*.

9. Press the Mode Key to overwrite all calibration data and to put the K3NH into RUN mode. The calibration data will not be overwritten if *no* is selected.

Set Value LED Display Model

Basic Model




RUN mode

5-3-7 Voltage Input Calibration

Preparation

Connect an STV to input terminals 12 and 14.


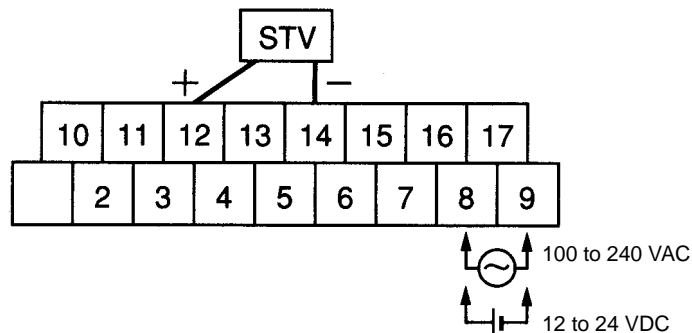


Calibration (0 to 5 V or 1 to 5 V)

- 1, 2, 3... 1. First, the *SURE* alarm display will appear. This will not appear once field calibration is performed.

Set Value LED Display Model



Basic Model



2. Press the Mode Key to display *1.5*. The teaching indicator will be lit.

Set Value LED Display Model



Basic Model



3. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of STV to 5 V. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



4. The display will change to *1.0* for 0-V calibration. The teaching indicator will be lit.

Set Value LED Display Model



Basic Model



5. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of STV to 0 V. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



6. The display will change to *5.0* for confirmation of the settings.

Set Value LED Display Model



Basic Model



7. Press the Shift Key to select whether or not to accept the settings.

Set Value LED Display Model



Basic Model



8. Press the Up Key to select *YES*.
9. Press the Mode Key to overwrite all calibration data and to put the K3NH into RUN mode. The calibration data will not be overwritten if *no* is selected.

Set Value LED Display Model

Basic Model



RUN mode



Calibration (0 to 10 V)

1, 2, 3...

1. First, the *SURE* alarm display will appear. This will not appear once field calibration is performed.

Set Value LED Display Model



Basic Model



2. Press the Mode Key to display *2u 10*. The teaching indicator will be lit.

Set Value LED Display Model



Basic Model



3. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of STV to 10 V. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model



Basic Model



4. The display will change to *2u 0* for 0-V calibration. The teaching indicator will be lit.


Set Value LED Display Model

Basic Model




5. Press the RESET/TEACH Key to display the calibration value setting. Then set the output of STV to 0 V. The teaching indicator will flash. After the value stabilizes (i.e., the fluctuation of the value is less than several digits), press the Mode Key to tentatively register the calibration data.

Set Value LED Display Model Basic Model




6. The display will change to *Str* for confirmation of the settings.

Set Value LED Display Model Basic Model




7. Press the Shift Key to select whether or not to accept the settings.

Set Value LED Display Model Basic Model



8. Press the Up Key to select *YES*.
9. Press the Mode Key to overwrite all calibration data and to put the K3NH into RUN mode. The calibration data will not be overwritten if *no* is selected.

Set Value LED Display Model Basic Model

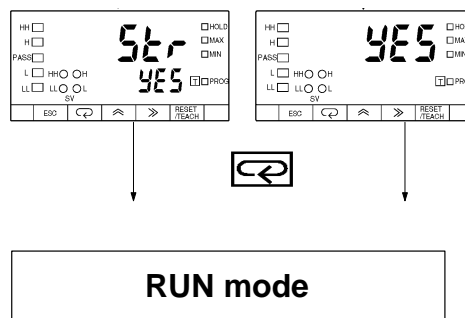

SECTION 6


BCD Output

This section provides information on the use of the K3NH with the BCD Output Board.

6-1	Connectors	94
6-2	Timing Charts	97

6-1 Connectors

Terminal Arrangement

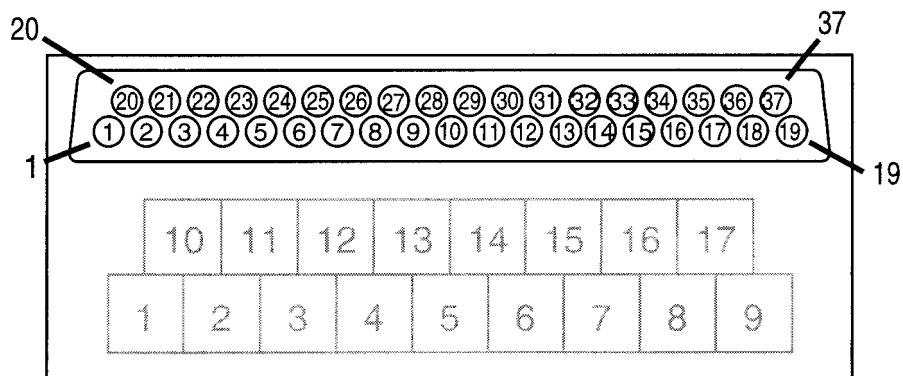

Terminal number	Signal name	Signal direction	Use
1	COM	---	GND:VO (See note 1.)
2	RD1-1	Output	1: Read data 10^0 digit
3	RD1-2	Output	2: Read data 10^0 digit
4	RD1-4	Output	4: Read data 10^0 digit
5	RD1-8	Output	8: Read data 10^0 digit
6	RD2-1	Output	1: Read data 10^1 digit
7	RD2-2	Output	2: Read data 10^1 digit
8	RD2-4	Output	4: Read data 10^1 digit
9	RD2-8	Output	8: Read data 10^1 digit
10	RD3-1	Output	1: Read data 10^2 digit
11	RD3-2	Output	2: Read data 10^2 digit
12	RD3-4	Output	4: Read data 10^2 digit
13	RD3-8	Output	8: Read data 10^2 digit
14	RD4-1	Output	1: Read data 10^3 digit
15	RD4-2	Output	2: Read data 10^3 digit
16	RD4-4	Output	4: Read data 10^3 digit
17	RD4-8	Output	8: Read data 10^3 digit
18	RD5-1	Output	1: Read data 10^4 digit
19	RD5-2	Output	2: Read data 10^4 digit
20	RD5-4	Output	4: Read data 10^4 digit
21	RD5-8	Output	8: Read data 10^4 digit
22	OVER	Output	Output when input value is not within the display range.
23	D - V	Output	Data confirmation signal
24	RUN	Output	Operation signal
25	COM	---	GND:VO (See note 1.)
26	REQ	Input	PV output request
27	MAX REQ	Input	Maximum value output request
28	MIN REQ	Input	Minimum value output request
29	HOLD	Input	Hold input
30	RESET	Input	Reset input
31	POL	Output	Positive/Negative polarity signal
32	HH	Output	HH output (See note 2.)
33	H	Output	H output (See note 2.)
34	PASS	Output	PASS output (See note 2.)
35	L	Output	L output (See note 2.)

Terminal number	Signal name	Signal direction	Use
36	LL	Output	LL output (See note 2.)
37	COM	Output	GND:VO (See note 1.)

- Note**
1. Terminals 1, 25, and 37 have the same COM.
 2. Refer to 2-3 *Output Board* for comparative outputs.

Applicable Connectors

Use the connector provided with the K3NH or an equivalent connector for the cable connecting to the BCD output connector.

The following connectors are provided with the K3NH.

Plug: XM2A-3701 (OMRON)

Hood: XM2S-3711 (OMRON)

The depth required for the installation of the K3NH is 200 mm min. in consideration of the space required by the cable.

Connecting Conditions

Refer to the following for the connecting conditions of each I/O. Refer to 2-3 *Output Block* for output signals HH through LL.

• Input

Input current with no voltage input: 10 mA

Signal level

ON voltage: 1.5 V max.

OFF voltage: 3 V min.


• Output

Rated load voltage: 24 VDC

Rated load current: 10 mA

Current leakage: 10 μ A max.

Connection Example

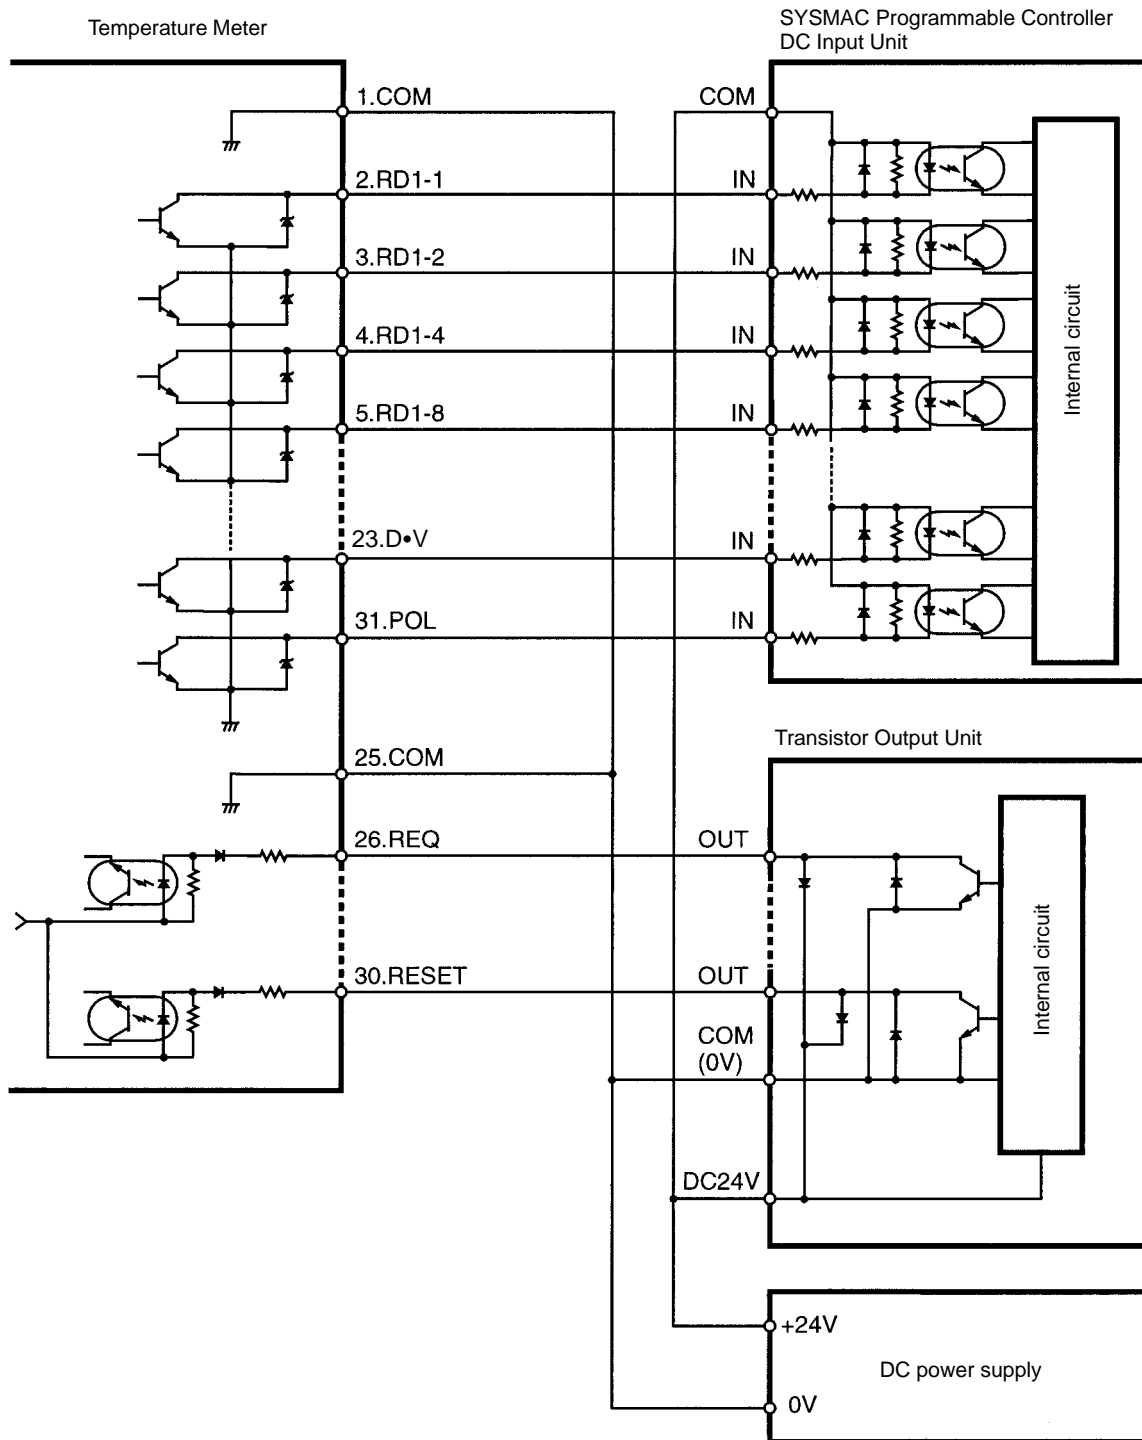

- Note**
1. Connect RD2-1 through RD2-4, RS3-1 through RS3-4, RD4-1 through RD4-4, and RD5-1 through RD5-4 in the same way as RD1-1 through RD1-4.
 2. Connect the RUN and OVER signals if they are used as status data.

Signals

When the HOLD signal is ON, the measurement operation stops and the process value input effective immediately before the HOLD signal is retained.

When the RESET signal is ON, the maximum and minimum values are set to the process value.

The OVER signal is ON when the input value is not within the display range.


The process value is output when the MAXREQ or MINREQ signal is ON at the time the output is tested in output test.

Multiple input signals must not turn ON. If multiple input signals turn ON or a single signal input is combined with another signal input, all output data will be turned OFF.


6-2 Timing Charts

When a REQ signal is input from a Programmable Controller to the K3NH in RUN or output test, the K3NH outputs a DATA VALID (D•V) signal. In other cases, the K3NH has All Signals OFF (H) output.

Refer to the following for the timing of each signal.

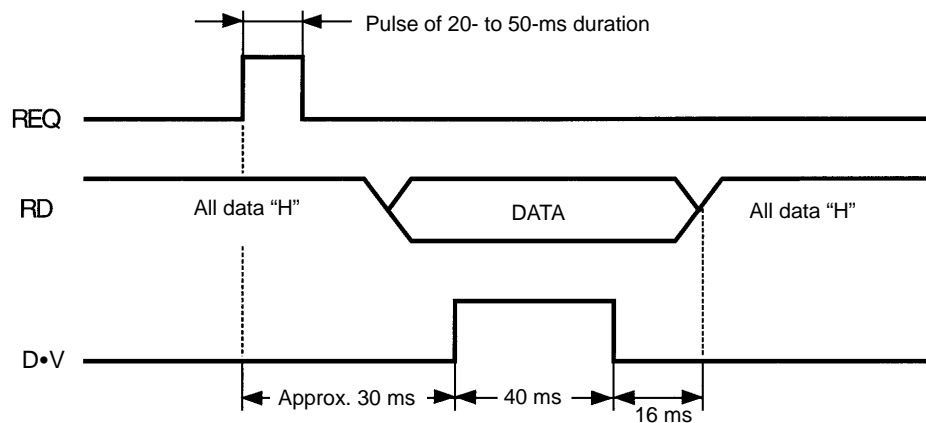

The REQ signal must be kept ON as shown below if the K3NH has continuous data output.

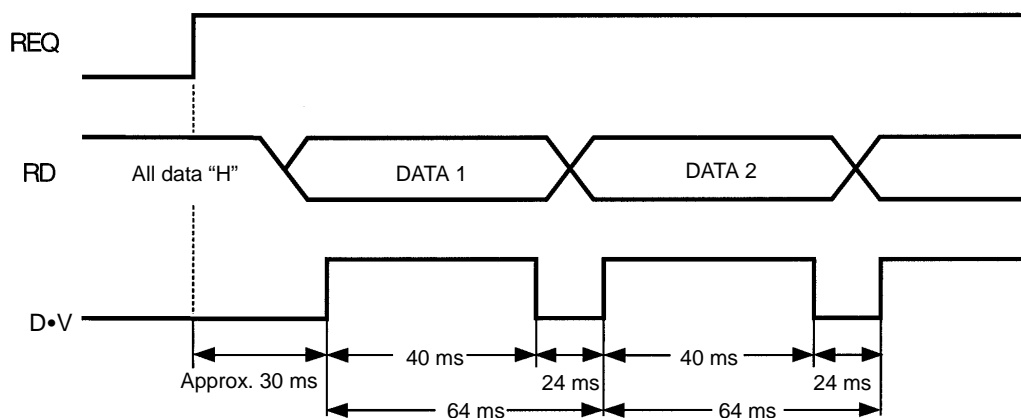

The polarity of the data must be checked with a POLARITY signal. The polarity is positive when the POLARITY signal is OFF and negative when the POLARITY signal is ON.

The K3NH in output test has test data output regardless of the type of REQ signal.

Operating Conditions

The RUN signal is turned ON in RUN or output test. The RUN signal is, however, turned OFF when an error other than overflow results.

Do not input multiple signals, otherwise all output data will be turned OFF.

SECTION 7

Troubleshooting

This section provides information for troubleshooting the K3NH.

7-1	Items to Be Checked First	100
7-2	Display	100
7-2-1	Flashing	100
7-2-2	Error Message	100

7-1 Items to Be Checked First

First, check the following three items if the K3NH has any problems during operation.

1, 2, 3...

1. Power Supply

Be sure that power supplied to the K3NH is within the rated voltage range.

2. Wiring

Be sure that the K3NH is wired correctly.

3. Communications Conditions

If the model is a K3NH with the Communications Output Board, be sure that the baud rate and unit numbers are correct.

After checking and remedying the above items, if the K3NH still has problems during operation, check the error message.

7-2 Display

7-2-1 Flashing

The display will flash in the following cases.

- The input or process value is not within the display range.

If the display flashes the output status will be as follows:

Models with BCD Output Board: The OVER signal will be ON.

Models with Communications Output Board: The OVER or UNDER signal will be ON and other output signals will be retained.

- The display will flash for three seconds if an attempt is made to change a setting on the K3NH. Set to remote programming to accept key input.

7-2-2 Error Message

The error condition can be checked with the error message.

The K3NH will have the following output statuses when an error message is displayed.

- HH, H, PASS, L, and LL will all be OFF.
- Linear output will be limited to the minimum value.
- The type of BCD output will be All Outputs OFF (H).
- The Unit error response will be returned from the model with a communications function.

$\bar{n}1.Err$

$\bar{n}2.Err$

$\bar{n}3.Err$

Memory Error

Meaning of Error

The internal memory has an error.

Remedy

Turn the K3NH off and on. If the memory error still exists, the K3NH will need to be repaired. If the K3NH returns to normal operation, the K3NH may have been affected by noise. Check if there is any source of noise generation near the K3NH.

$\bar{Ad}.Err$

AD Converter Error

Meaning of Error

The internal circuit has an error.

Remedy

Turn the K3NH off and on. If the AD converter error still exists, the K3NH will need to be repaired. If the K3NH returns to normal operation, the K3NH may have been affected by noise. Check if there is any source of noise generation near the K3NH.

Err- $\bar{0}$ CHG- $\bar{0}$ **Output Error****Meaning of Error**

The internal circuit has an error.

Remedy

Turn the K3NH off and on. If the output error still exists, the K3NH will need to be repaired.

S.Err

Sensor Error**Meaning of Error**

The input has an error.

The input to the Sensor is outside the measurement range.

Remedy

Check for input wiring errors, wire breakage, short circuits, and input type.

Check the input temperature and the measurement range of the Sensor. If the temperature is outside the measurement range, replace the Sensor so that the input temperature will fall within its measurement range.

Appendix A

Specifications

Ratings

Supply voltage	100 to 240 VAC (50/60 Hz); 12 to 24 VDC
Operating voltage range	85% to 110% of supply voltage
Power consumption (see note)	15 VA max. (max. AC load with all indicators lit) 10 W max. (max. DC load with all indicators lit)
Insulation resistance	20 M Ω min. (at 500 VDC) between external terminal and case. Insulation provided between inputs, outputs, and power supply.
Dielectric withstand voltage	2,000 VAC for 1 min between external terminal and case. Insulation provided between inputs, outputs, and power supply.
Noise immunity	$\pm 1,500$ V on power supply terminals in normal or common mode ± 1 μ s, 100 ns for square-wave noise with 1 ns
Vibration resistance	Malfunction: 10 to 55 Hz, 0.5-mm for 10 min each in X, Y, and Z directions Destruction: 10 to 55 Hz, 0.75-mm for 2 hrs each in X, Y, and Z directions
Shock resistance	Malfunction: 98 m/s ² (10G) for 3 times each in X, Y, and Z directions Destruction: 294 m/s ² (30G) for 3 times each in X, Y, and Z directions
Ambient temperature	Operating: -10°C to 55°C (with no icing) Storage: -20°C to 65°C (with no icing)
Ambient humidity	Operating: 25% to 85% (with no condensation)
Ambient atmosphere	Must be free of corrosive gas
EMC	Emission Enclosure: EN55011 Group 1 class A Emission AC Mains: EN55011 Group 1 class A Immunity ESD: EN61000-4-2: 4-kV contact discharge (level 2) 8-kV air discharge (level 3) Immunity-RF-interference: ENV50140: 10 V/m (amplitude modulated, 80 MHz to 1 GHz) (level 3) 10 V/m (pulse modulated, 900 MHz) Immunity Conducted Disturbance: ENV50141: 10 V (0.15 to 80 MHz) (level 3) Immunity Burst: EN61000-4-4: 2-kV power-line (level 3) 2-kV I/O signal-line (level 4)
Approved standards	UL508, CSA22.2; conforms to EN50081-2, EN50082-2, EN61010-1 (IEC1010-1); conforms to VDE106/part 100 (Finger Protection) when the terminal cover is mounted.
Weight	Approx. 400 g

Note An Intelligent Signal Processor with DC supply voltage requires approximately 1 A DC as control power supply current the moment the Intelligent Signal Processor is turned on. Do not forget to take this into consideration when using several Intelligent Signal Processors. When the Intelligent Signal Processor is not in measuring operation (e.g., the Intelligent Signal Processor has been just turned on or is operating for start-up compensation time), the display will read "00000" and all outputs will be OFF.

Input/Output Ratings

Relay Contact Output

(Incorporating a G6B Relay)

Item	Resistive load ($\cos\phi = 1$)	Inductive load ($\cos\phi = 0.4$, $L/R = 7$ ms)
Rated load	5 A at 250 VAC; 5 A at 30 VDC	1.5 A at 250 VAC, 1.5 A at 30 VDC
Rated carry current	5 A max. (at COM terminal)	
Max. contact voltage	380 VAC, 125 VDC	
Max. contact current	5 A max. (at COM terminal)	
Max. switching capacity	1,250 VA, 150 W	375 VA, 80 W
Min. permissible load (P level, reference value)	10 mA at 5 VDC	
Mechanical life	50,000,000 times min. (at a switching frequency of 18,000 times/hr)	
Electrical life (at an ambient temperature of 23°C)	100,000 times min. (at a rated load switching frequency of 1,800 times/hr)	

Transistor Output

Rated load voltage	12 to 24 VDC $+10\%/ -15\%$
Max. load current	50 mA
Leakage current	100 μ A max.

BCD Output

I/O signal name		Item	Rating
Inputs	REQUEST, HOLD, MAX, MIN, RESET	Input signal	No-voltage contact input
		Input current with no-voltage input	10 mA
		Signal level	ON voltage: 1.5 V max. OFF voltage: 3 V min.
Outputs	DATA, POLARITY, OVERFLOW, DATA VALID, RUN	Rated load voltage	12 to 24 VDC $+10\%/ -15\%$
		Max. load current	10 mA
		Leakage current	100 μ A max.

Note Logic method: negative logic

Linear Output

Item	4 to 20 mA	1 to 5 V	1 mV/10 digits (see note)
Resolution	4,096		
Output error	$\pm 0.5\%$ FS		$\pm 1.5\%$ FS
Permissible load resistance	600 Ω max.	500 Ω min.	1 K Ω min.

Note For the 1 mV/10-digit output, the output voltage changes for every 40 to 50 increment in the display value.

Communications

Item		RS-232C, RS-422	RS-485
Transmission method		4-wire, half-duplex	2-wire, half-duplex
Synchronization method		Start-stop synchronization	
Baud rate		1,200/2,400/4,800/9,600/19,200/38,400 bps	
Transmission code		ASCII (7-bit)	
Communications	Write to K3NH	Comparative set value, prescaling value, remote/local programming, reset control of maximum/minimum values, and other setting mode items excluding communications conditions.	
	Read from K3NH	Process value, comparative set value, maximum value, minimum value, model data, error code, and others	

For details, refer to *Communication Operation Manual*.

Characteristics

Indication accuracy (at 23±5°C) (see note)	Thermocouple: (±0.3% of indication value or ±1°C, whichever greater) ±1 digit max. Platinum resistance thermometer: (±0.2% of indication value or ±0.8°C, whichever greater) ±1 digit max. Analog input: ±0.2% FS ±1 digit max.
Input	Thermocouple: K, J, T, E, L, U, N, R, S, B, W, PLII Platinum resistance thermometer: JPt100, Pt100 Current input: 4 to 20 mA, 0 to 20 mA Voltage input: 1 to 5 V, 0 to 5 V, 0 to 10 V
Sampling period	Temperature input: 250 ms Analog input: 100 ms
Input shift	Two-point settings (upper limit and lower limit)
Max. displayed digits	5 digits (–19999 to 99999)
Display	7-segment LED
Polarity display	“–” is displayed automatically with a negative input signal.
Zero display	Leading zeros are not displayed.
HOLD function	Maximum hold (maximum data) Minimum hold (minimum data)
External controls	HOLD: (Process value held) RESET: (Maximum/Minimum data reset)
Comparative output hysteresis setting	Programmable with front-panel key inputs (1 to 9999).
Other functions	Variable linear output range (for models with linear outputs only) Remote/Local processing (available for communications output models only) Maximum/Minimum value data reset with front panel keys °C/°F display selection Averaging processing function (simple or moving average) Comparative output pattern selection Standby sequence Security Field calibration
Output configuration	Relay contact output (5 outputs) Transistor output (NPN and PNP open collector), BCD (NPN open collector) Parallel BCD (NPN open collector) + transistor output (NPN open collector) Linear output (4 to 20 mA, 1 to 5 V) + transistor output (NPN open collector) Communication functions (RS-232C, RS-485, RS-422) Communication functions (RS-232C, RS-485, RS-422) + transistor output (NPN open collector)
Delay in comparative outputs (transistor output)	500 ms max.
Enclosure rating	Front panel: NEMA4 for indoor use (equivalent to IP66) Rear case: IEC standard IP20 Terminals: IEC standard IP00
Memory protection	Non-volatile memory (EEPROM) (possible to rewrite 100,000 times)

Note The indication accuracy of the K1, T, and N thermocouples at a temperature of -100°C or less is ±2°C ±1 digit maximum. The indication accuracy of the U, L1, and L2 thermocouples at any temperature is ±2°C ±1 digit maximum.

The indication accuracy of the B thermocouple at a temperature of 400°C or less is unrestricted.

The indication accuracy of the R and S thermocouples at a temperature of 200°C or less is ±3°C ±1 digit maximum.



The indication accuracy of the W thermocouple at any temperature is (±0.3% of the indicated value or ±3°C, whichever is greater) ±1 digit maximum.

The indication accuracy of the PLII thermocouple at any temperature is (±0.3% or ±2°C, whichever is greater) ±1 digit maximum.

Appendix B

Available Models

Base Units

Model	Supply voltage	
	100 to 240 VAC	12 to 24 VDC
Basic Models These models provide a present value LED and front-panel control keys. Can be connected to any Output Board, or can be used for display only without an Output Board. 	K3NH-TA1A	K3NH-TA2A
Set Value LED Models These models provide a present value LED, set value LED, and front-panel control keys. Can be connected to Relay, Transistor, or Combination Output Boards. 	K3NH-TA1C	K3NH-TA2C

Available Output Board Combinations

Output type	Output configuration	Output boards	Base units	
			Basic	Set Value LED Display
Relay contact	3 outputs: H, PASS, L (SPDT)	K31-C1	Yes	Yes
	5 outputs: HH, H, L, LL (SPST-NO), and PASS (SPDT)	K31-C2	Yes	Yes
	5 outputs: HH, H, L, LL (SPST-NC), and PASS (SPDT)	K31-C5	Yes	Yes
Transistor	5 outputs (NPN open collector)	K31-T1	Yes	Yes
	5 outputs (PNP open collector)	K31-T2	Yes	Yes
BCD (see note)	5-digit output (NPN open collector)	K31-B2	Yes	---
Linear	4 to 20 mA DC	K31-L1	Yes	---
	1 to 5 VDC	K31-L2	Yes	---
	1 mV/10 digits	K31-L3	Yes	---
	0 to 5 VDC	K31-L7	Yes	---
	0 to 10 VDC	K31-L8	Yes	---
Communication boards (see note)	RS-232C	K31-FLK1	Yes	---
	RS-485	K31-FLK2	Yes	---
	RS-422	K31-FLK3	Yes	---
Combination output and communication boards	BCD output + 5 transistor outputs (NPN open collector)	K31-B4	Yes	Yes
	4 to 20 mA + 5 transistor outputs (NPN open collector)	K31-L4	Yes	Yes
	1 to 5 V + 5 transistor outputs (NPN open collector)	K31-L5	Yes	Yes
	1 mV/10 digits + 5 transistor outputs (NPN open collector)	K31-L6	Yes	Yes
	0 to 5 VDC + 5 transistor outputs (NPN open collector)	K31-L9	Yes	Yes
	0 to 10 VDC + 5 transistor outputs (NPN open collector)	K31-L10	Yes	Yes
	RS-232C + 5 transistor outputs (NPN open collector)	K31-FLK4	Yes	Yes
	RS-485 + 5 transistor outputs (NPN open collector)	K31-FLK5	Yes	Yes
	RS-422 + 5 transistor outputs (NPN open collector)	K31-FLK6	Yes	Yes

Note For details, refer to the *Communication Operation Manual*.

Model Number Legend

Base Units and Output Boards can be ordered individually or as sets. Refer to the Available Output Board Combinations table on page 107.

Base Units

K3NH -
 1 2 3 4

Output Boards

K31 -
 5 6 7 8

Base Units with Output Boards

K3NH - -
 1 2 3 4 5 6 7 8

1, 2. Input Sensors Codes

TA: Current series

3. Supply Voltage

1: 100 to 240 VAC

2: 12 to 24 VDC

4. Display

A: Basic

C: Set Value LED Display

5, 6, 7, 8. Output Type Codes

C1: 3 comparative relay contact outputs (H, PASS, L: SPDT)

C2: 5 comparative relay contact outputs (HH, H, L, LL: SPST-NO; PASS: SPDT)

C5: 5 comparative relay contact outputs (HH, H, L, LL: SPST-NC; PASS: SPDT)

T1: 5 comparative transistor outputs (NPN open collector)

T2: 5 comparative transistor outputs (PNP open collector)

B2: BCD output (NPN open collector) (see note)

B4: BCD output + 5 transistor outputs (NPN open collector)

L1: Linear output (4 to 20 mA) (see note)

L2: Linear output (1 to 5 VDC) (see note)

L3: Linear output (1 mV/10 digits) (see note)

L4: Linear output, 4 to 20 mA + 5 transistor outputs (NPN open collector)

L5: Linear output, 1 to 5 V + 5 transistor outputs (NPN open collector)

L6: Linear output, 1 mV/10 digits+ 5 transistor outputs (NPN open collector)

L7: Linear output, 0 to 5 VDC (see note)

L8: Linear output, 0 to 10 VDC (see note)

L9: Linear output, 0 to 5 VDC + 5 transistor outputs (NPN open collector)

L10: Linear output, 0 to 10 VDC + 5 transistor outputs (NPN open collector)

FLK1: Communication RS-232C (see note)

FLK2: Communication RS-485 (see note)

FLK3: Communication RS-422 (see note)

FLK4: RS-232C + 5 transistor outputs (NPN open collector)

FLK5: RS-485 + 5 transistor outputs (NPN open collector)

FLK6: RS-422 + 5 transistor outputs (NPN open collector)

Note These output types are available on Basic Models only.

Appendix C

List of Settings

Use this sheet to keep a record of set values.

Menu	Parameter	Setting range	Unit	Set value
5u5Et Setting value menu	5u.HH HH set value	–1999 to 9,999	---	
	5u. H H set value	–1999 to 9,999	---	
	5u. L L set value	–1999 to 9,999	---	
	5u.LL LL set value	–1999 to 9,999	---	
5EtUP Setup menu	Ln-t Input type	JPt100, Pt100, K1, K2, J1, J2, T, E, L1, L2, U, N, R, S, B, W, PLII, 4 to 20 mA, 0 to 20 mA, 1 to 5 V, 0 to 5 V, 0 to 10 V	---	
	Ln-F °C/°F display change	°C/°F	---	
	Ln-H Scaling upper limit value	–1999 to 9,999		
	Ln-L Scaling lower limit value	–1999 to 9,999		
	dEE-P Decimal point position	0000/0.000/00.00/000.0		
	U-nō Communications unit no.	0 to 99	---	
	bPS Baud rate	1,200/2,400/4,800/9,600/19,200/38,400	bps	
	LEn Word length	7/8	bit	
	SbLt Stop bits	1/2	bit	
	PrLy Parity bits	None/Even/Odd	---	
ōPt Option menu	AvG Average processing	No average processing Movement average processing times: 2, 4, 8, 16, or 32 times Simple average processing times: 2, 4, 8, 16, or 32 times	---	
	dLGLt Display digit change	4/5 digits	---	
	LnSH Upper-limit temperature input compensation value	–1999 to 9,999	---	
	LnSL Lower-limit temperature input compensation value	–1999 to 9,999	---	
	HLS Hysteresis	1 to 9,999	---	
	LnōUt Comparative output pattern	Standard, zone, or level output	---	
	StdbY Standby sequence	ON/OFF	---	
	LSEt.H H linear output range	–1999 to 9,999	---	
	LSEt.L L linear output range	–1999 to 9,999	---	
	r-L Remote/Local processing	Remote/Local	---	

Appendix D

Available Parameters

Available parameters vary with the output board of the K3NH and are indicated as “YES” in the following table.

Setting Mode

Menu	Parameter		Output board								
			No output	C1	C2/C5 /T1/T2	B2	B4	L1/L2/ L3/ L7/L8	L4/L5/ L6/L9/ L10	FLK1/ FLK2/ FLK3	FLK4/ FLK5/ FLK6
S _u SEt Setting value menu	S _u .HH	HH set value			YES		YES		YES		YES
	S _u . H	H set value		YES	YES		YES		YES		YES
	S _u . L	L set value		YES	YES		YES		YES		YES
	S _u .LL	LL set value			YES		YES		YES		YES
SEtUP Setup menu	ĩn-t	Input type	YES	YES	YES	YES	YES	YES	YES	YES	YES
	[-F	°C/°F display change	YES	YES	YES	YES	YES	YES	YES	YES	YES
	ĩn-H	Scaling upper limit value	YES	YES	YES	YES	YES	YES	YES	YES	YES
	ĩn-L	Scaling lower limit value	YES	YES	YES	YES	YES	YES	YES	YES	YES
	dEE-P	Decimal point position	YES	YES	YES	YES	YES	YES	YES	YES	YES
	U-nō	Communications unit no.								YES	YES
	bPS	Baud rate								YES	YES
	LEn	Word length								YES	YES
	Sbĭt	Stop bits								YES	YES
	Prty	Parity bits								YES	YES
ōPt Option menu	AvG	Average processing	YES	YES	YES	YES	YES	YES	YES	YES	YES
	dĭGĭt	Display digit change	YES	YES	YES	YES	YES	YES	YES	YES	YES
	ĩnSH	Upper-limit compensation value	YES	YES	YES	YES	YES	YES	YES	YES	YES
	ĩnSL	Lower-limit compensation value	YES	YES	YES	YES	YES	YES	YES	YES	YES
	HYS	Hysteresis		YES	YES		YES		YES		YES
	[-ōUt	Comparative output pattern		YES	YES		YES		YES		YES
	StdbY	Standby sequence		YES	YES		YES		YES		YES
	LSEt.H	H linear output range						YES (see note)	YES (see note)		
	LSEt.L	L linear output range						YES (see note)	YES (see note)		
	r-L	Remote or Local processing								YES	YES

Note The linear output range cannot be set with the K31-L3 and K31-L6 Output Boards.

Protect Mode

Menu	Parameter		Output board								
			No output	C1	C2/C5 /T1/T2	B2	B4	L1/L2/ L3/L7/ L8	L4/L5/ L6/L9/ L10	FLK1/ FLK2/ FLK3	FLK4/ FLK5/ FLK6
Protect menu	RLl	All key protect	YES	YES	YES	YES	YES	YES	YES	YES	YES
	SuSEt	Set value change prohibit		YES	YES		YES		YES		YES
	ññ.rSt	Maximum/Minimum value clear prohibit	YES	YES	YES	YES	YES	YES	YES	YES	YES
	SECr	Security	YES	YES	YES	YES	YES	YES	YES	YES	YES

Index

A

AD converter error, 100
All Key Protect, setting, 60
average processing, description, 3
average processing, settings, 39

B

Base Unit, available models, 107
baud rate, setting, 34
BCD output, ratings, 104
BCD Output Boards
 connectors, 94
 operation, 93
 timing charts, 97

C

calibration, field calibration, 8
calibration
 current input calibration, 88
 field calibration, 78
 thermocouple calibration, 79
 thermometer calibration, 85
 voltage input calibration, 89
characteristics, 105
chattering
 preventing, 46
 prevention, 46
combination output boards, 16
communications, ratings, 104
communications format, setting, 36
communications function, 8
communications unit number, setting, 34
comparative output pattern, setting, 48
comparative output selection, description, 2
comparative outputs, setting, 49
current input, wiring, 13
current inputs, calibration, 88
current–input calibration, 88

D

decimal point position, setting, 31
default settings, initialization of set values, 77
digits, changing number of digits displayed, 42
dimensions, 10
display
 description, 3
 troubleshooting, 100
display digits, changing, 42

E–F

error messages, 100
external control inputs, 13
external input signals, operation, 72
field calibration, 8
field calibration, 78
flashing display, 100

H

HOLD input, wiring, 13
HOLD input, 72
 description, 2
host computer, unit number setting, 34
hysteresis setting, setting, 46
hysteresis setting, description, 2

I

indicators, description, 3
Initialization, of set values, 77
Input Block, 11
input type, setting, 27

L

LED indicators, description, 3
level output, 49
linear output, ratings, 104
linear output boards, 17
linear output range, setting, 53
linear output range, teaching, 75
local programming, setting, 56
lower–limit compensation value, setting, 44

M

- Maintenance mode, 8
- Maintenance mode, operation, 77
- maximum values
 - displaying and resetting, 71
 - protecting, 63
- measurement ranges, for temperature inputs, 12
- memory error, 100
- menu overview
 - Protect mode, 59
 - Setting mode, 22
- menus
 - option menu, 39
 - protect menu, 60
 - setting value menu, 23
 - setup menu, 27
- minimum values
 - displaying and resetting, 71
 - protecting, 63
- model numbers, meaning, 108
- models, standard models, 107
- modes, operating modes, 7
- mounting method, 11

O

- operation keys, description, 3
- option menu, 39
- output board, 14
- Output Boards
 - available models, 107
 - available parameters, 111
- output error, 101
- output test, operation, 76
- output test function, description, 2

P

- panel cutouts, 10
- parameter settings, 19
 - procedures, 20
- parameters
 - available in each Output Board, 111
 - list, 109
- parity bits, setting, 36
- PASS output, 48

- Power Supply, wiring, 12
- precautions
 - general, xi
 - wiring, 12
- protect menu, 60
- Protect mode, 8
- Protect mode, 58
 - selecting, 58

R

- ratings, 103
- relay contact output, ratings, 104
- relay output boards, 16
- remote/local programming, setting, 56
- remote/local selection, description, 2
- RESET input, wiring, 13
- RESET input, 72
 - description, 2
- RUN mode, 7
- RUN mode, operations, 67

S

- scaling, description, 2
- scaling
 - setting lower limit value, 31
 - setting upper limit value, 31
- Security, setting, 65
- sensor error, 101
- set value, teaching, 74
- set value menu, 23
- set values, 23
 - changing, 68
 - displaying, 68
 - initializing, 77
 - protecting, 61
 - setting ranges, 23
- Setting mode, 8
- Setting mode, 21
 - selecting, 21
- Setting Value Change Prohibit, setting, 61
- settings
 - list, 109
 - protecting, 65
- setup, 9
- setup menu, 27
- specifications, 103
- standard models, 107
- standard output, 48

standby sequence, description, 2
standby sequence, setting, 51
stop bits, setting, 36

T

teaching, description, 2
teaching function, operation, 74
temperature inputs
 setting upper limit compensation value, 44
 wiring, 12
temperature units, setting, 29
temperature–resistance thermometer, 85
terminal arrangement
 BCD Output Boards, 94
 Input Block, 11
 output board, 14
terminal arrangement, 6

thermocouple calibration, 79
thermometer calibration, 85
timing charts, for BCD Output Boards, 97
transistor output, ratings, 104
transistor output boards, 16
troubleshooting, 99


U–Z

unit number, setting, 34
upper–limit compensation value, setting, 44
voltage input, wiring, 13
voltage inputs, calibration, 89
voltage–input calibration, 89
wiring, 12
word length, setting, 36
zone output, 49

Revision History

A manual revision code appears as a suffix to the catalog number on the front cover of the manual.

Cat. No. N92-E1-1



Revision code

The following table outlines the changes made to the manual during each revision. Page numbers refer to the previous version.

Revision code	Date	Revised content
1	January 1998	Original production